

## Event Generator

**cPCI-EVG-220, cPCI-EVG-230, cPCI-EVG-300,**

**PXIe-EVG-300 and VME-EVG-230**

**Modular Register Map Firmware Version 0006**

## Contents

Safety Summary .....	4
Ground the Equipment. ....	4
Keep away From Live Circuits inside the Equipment. ....	4
Do Not Substitute Parts or Modify Equipment. ....	4
Flammability .....	4
EMI Caution .....	4
CE Notice .....	4
Hardware Installation .....	6
Installing the 3U Boards (cPCI-EVG-2x0 or PXIe-EVG-300) into a Chassis .....	6
Installing the 6U Boards (VME-EVG-230 or cPCI-EVG-300) into a Chassis .....	6
Replacing SFP (Small Form Factor Pluggable) Transceivers .....	6
Introduction .....	9
Event Stream Details .....	9
Event Codes.....	9
Distributed Bus and Data Transmission .....	10
Event Sources .....	10
Trigger Events .....	10
Upstream Events.....	11
Event Sequencer .....	12
Distributed Bus.....	13
Timestamping Inputs .....	14
Timestamp Generator.....	14
Multiplexed Counters .....	15
Configurable Size Data Buffer .....	15
Programmable Front Panel Connections .....	17
AC Line Synchronisation .....	17
Event Clock .....	17
RF Clock and Event Clock .....	18
Fractional Synthesiser .....	19
Connections .....	20
cPCI-EVG-2x0 Front Panel Connections.....	20
VME-EVG-230 Front Panel Connections.....	21
VME-EVG-230 VME P2 User I/O Pin Configuration.....	22

cPCI-EVG-300 Front Panel Connections.....	22
PXIe-EVG-300 Front Panel Connections .....	23
PXIe-EVG-300 Backplane Connections .....	23
Programming Details.....	25
VME-EVG-230 CR/CSR Support.....	25
Function 0/1/2 Registers.....	25
VME-EVG-230 Network Interface .....	27
Assigning an IP Address to the Module .....	27
Using Telnet to Configure Module.....	27
Boot Configuration (command b) .....	27
Memory dump (command d).....	28
Memory modify (commands d and m).....	28
Upgrading IP2022 Microprocessor Software (command u).....	29
Linux .....	29
Windows.....	29
Upgrading FPGA Configuration File .....	29
Linux .....	29
Windows.....	29
Linux .....	30
Windows.....	30
UDP Remote Programming Protocol .....	30
Read Access (Type 0x01).....	31
Write Access (Type 0x02).....	31
Register Map .....	32
Application Programming Interface (API).....	48
Function Reference.....	48
int EvgOpen(struct MrfEgRegs **pEg, char *device_name); .....	48
int EvgClose(int fd); .....	49
int EvgEnable(volatile struct MrfEgRegs *pEg, int state); .....	49
int EvgGetEnable(volatile struct MrfEgRegs *pEg); .....	49
int EvgRxEnable(volatile struct MrfEgRegs *pEg, int state); .....	49
int EvgRxGetEnable(volatile struct MrfEgRegs *pEg); .....	49
int EvgGetViolation(volatile struct MrfEgRegs *pEg, int clear); .....	50
int EvgSWEEventEnable(volatile struct MrfEgRegs *pEg, int state); .....	50
int EvgGetSWEEventEnable(volatile struct MrfEgRegs *pEg); .....	50
int EvgSendSWEEvent(volatile struct MrfEgRegs *pEg, int code); .....	50
int EvgEvanEnable(volatile struct MrfEgRegs *pEg, int state); .....	50
int EvgEvanGetEnable(volatile struct MrfEgRegs *pEg); .....	51
void EvgEvanReset(volatile struct MrfEgRegs *pEg); .....	51
void EvgEvanResetCount(volatile struct MrfEgRegs *pEg); .....	51
int EvgEvanGetEvent(volatile struct MrfEgRegs *pEg, struct EvanStruct *evan); .....	51
int EvgSetMXCPrescaler(volatile struct MrfEgRegs *pEg, int mxc, unsigned int presc); ..	51
int EvgSetMxcTrigMap(volatile struct MrfEgRegs *pEg, int mxc, int map); .....	52
void EvgSyncMxc(volatile struct MrfEgRegs *pEg); .....	52
void EvgMXCDump(volatile struct MrfEgRegs *pEg); .....	52
int EvgSetDBusMap(volatile struct MrfEgRegs *pEg, int dbus, int map); .....	52
void EvgDBusDump(volatile struct MrfEgRegs *pEg); .....	52

int EvgSetACInput(volatile struct MrfEgRegs *pEg, int bypass, int sync, int div, int delay);	53
.....	
int EvgSetACMap(volatile struct MrfEgRegs *pEg, int map);	53
void EvgACDump(volatile struct MrfEgRegs *pEg);	53
int EvgSetRFInput(volatile struct MrfEgRegs *pEg, int useRF, int div);	53
int EvgSetFracDiv(volatile struct MrfEgRegs *pEg, int fracdiv);	54
int EvgSetSeqRamEvent(volatile struct MrfEgRegs *pEg, int ram, int pos, unsigned int timestamp, int code);	54
void EvgSeqRamDump(volatile struct MrfEgRegs *pEg, int ram);	54
int EvgSeqRamControl(volatile struct MrfEgRegs *pEg, int ram, int enable, int single, int recycle, int reset, int trgsel);	54
int EvgSeqRamSWTrig(volatile struct MrfEgRegs *pEg, int trig);	55
void EvgSeqRamStatus(volatile struct MrfEgRegs *pEg, int ram);	55
int EvgSetUnivinMap(volatile struct MrfEgRegs *pEg, int univ, int trig, int dbus);	55
void EvgUnivinDump(volatile struct MrfEgRegs *pEg);	55
int EvgSetTriggerEvent(volatile struct MrfEgRegs *pEg, int trigger, int code, int enable);	55
void EvgTriggerEventDump(volatile struct MrfEgRegs *pEg);	56
int EvgSetUnivOutMap(volatile struct MrfEgRegs *pEg, int output, int map);	56
int EvgSetDBufMode(volatile struct MrfEgRegs *pEg, int enable);	56
int EvgGetDBufStatus(volatile struct MrfEgRegs *pEg);	56
int EvgSendDBuf(volatile struct MrfEgRegs *pEg, char *dbuf, int size);	57

## **Safety Summary**

The following general safety precautions must be observed during all phase of operation, service and maintenance of this equipment. Failure to comply with these precautions could result in personal injury or damage to the equipment.

### ***Ground the Equipment.***

To minimize shock hazard, the equipment chassis and enclosure must be connected to an electrical ground.

### ***Keep away From Live Circuits inside the Equipment.***

Operating personnel must not remove equipment covers. Only Factory Authorized Service Personnel or other qualified service personnel may remove equipment covers for internal subassembly or component replacement or any internal adjustment. Service personnel should not replace components with power cable connected.

Avoid touching areas of integrated circuitry; static discharge can damage the equipment.

Use of an antistatic wrist strap is recommended when installing a system.

### ***Do Not Substitute Parts or Modify Equipment.***

Do not install substitute parts or perform any unauthorized modification of the equipment. Contact Micro-Research Finland for service and repair.

## **Flammability**

All Micro-Research Finland Oy PCBs (Printed Circuit Boards) are manufactured with a flammability rating of 94V-0 by UL-recognized manufacturers.

## **EMI Caution**

This equipment generates, uses and can radiate electromagnetic energy. It may cause or be susceptible to electromagnetic interference (EMI) if not installed and used with adequate EMI protection.

## **CE Notice**

This is a Class A product. In a domestic environment, this product may cause radio interference, in which case the user may be required to take adequate measures.

This product has been designed to comply with the essential requirement of the following European Directives:

Electromagnetic Compatibility (EMC) Directive 2004/108/EC, Low-Voltage Directive 2006/95/EC.

Conformity is assessed in accordance to the following standards:

EN55022 “Limits and Methods of Measurement of Radio Interference Characteristics of Information Technology Equipment”; Equipment Class A

EN60950-1 (Safety)

Laser Eye Safety and Equipment Type Testing (Avago AFBR-57R5APZ transceivers):  
(IEC) EN60825.1: 1994 + A11 + A2, (IEC) EN60825-2: 1994 + A1, (IEC) EN60950: 1992 + A1  
+ A2 + A3 + A4 + A11

## Hardware Installation

### ***Installing the 3U Boards (cPCI-EVG-2x0 or PXle-EVG-300) into a Chassis***

Use the following steps to install the module into the chassis:

1. Attach ESD strap to your wrist. Attach the other end of the ESD strip to an electrical ground. The ESD strip must be secured to your wrist and to ground throughout the procedure.
2. Remove the filler panel for the slot you want to mount the board into.
3. Unpack the board you want to install from its ESD bag.
4. Open handle by pushing grey levers. The fastening screw in the handle may have turned during transportation and prevent the handle from opening completely. Please use a screwdriver and turn screw clockwise if the handle does not open properly.
5. Install the top and bottom edge of the board into the guide rails of the chassis.
6. Slide the board into the slot until resistance is felt.
7. Use handle to insert board into slot. Simultaneously help slightly from the upper area of the front panel close to the countersunk screw. Do not push the board in using any other area of the front panel.
8. Make sure handle is in locked position (closed) and grey lever have clicked into the locked position.
9. Secure the board using the screw in the handle and top of board.
10. Connect appropriate cables to the board.

### ***Installing the 6U Boards (VME-EVG-230 or cPCI-EVG-300) into a Chassis***

Use the following steps to install the module into the chassis:

1. Attach ESD strap to your wrist. Attach the other end of the ESD strip to an electrical ground. The ESD strip must be secured to your wrist and to ground throughout the procedure.
2. Remove the filler panel for the slot you want to mount the board into.
3. Unpack the board you want to install from its ESD bag.
4. Open handles by pushing grey levers. Fastening screws in the handles may have turned during transportation and prevent the handles from opening completely. Please use a screwdriver and turn screws clockwise if the handles do not open properly.
5. Install the top and bottom edge of the board into the guide rails of the chassis.
6. Slide the board into the slot until resistance is felt.
7. Use handles to insert board into slot. Do not push the board in using the front panel.
8. Make sure handles are in locked position (closed) and grey levers have clicked into the locked position.
9. Secure the board using the screws in the handles
10. Connect appropriate cables to the board.

### ***Replacing SFP (Small Form Factor Pluggable) Transceivers***

SFP Transceivers are hot-pluggable and replaceable during operation. To replace a SFP transceiver use the following steps:

1. Attach ESD strap to your wrist. Attach the other end of the ESD strip to an electrical ground. The ESD strip must be secured to your wrist and to ground throughout the procedure.
2. Unplug any fibres connected to the transceiver you want to replace.
3. Pull out the transceiver using the transceiver handle that folds down.
4. Plug in a new transceiver.
5. Reconnect fibres.



## Introduction

The Event Generator is responsible of creating and sending out timing events to an array of Event Receivers. High configurability makes it feasible to build a whole timing system with a single Event Generator without external counters etc.

Events are sent out by the event generator as event frames (words) which consist of an eight bit event code and an eight bit distributed bus data byte. The event transfer rate is derived from an external RF clock or optionally an on-board clock generator. The optical event stream transmitted by the Event Generator is phase locked to the clock reference.

There are several sources of events: trigger events, sequence events, software events and events received from an upstream Event Generator. Events from different sources have different priority which is resolved in a priority encoder.

In addition to events the Event Generator enables the distribution of eight simultaneous signals sampled with the event clock rate, the distributed bus. Distributed bus signals may be provided externally or generated on-board by programmable multiplexed counters.

## Event Stream Details

The structure of the event stream is described to help understand the functioning of the event system. The event stream should be considered as a continuous flow of event frames which consist of two bytes, the event code and distributed bus data byte.

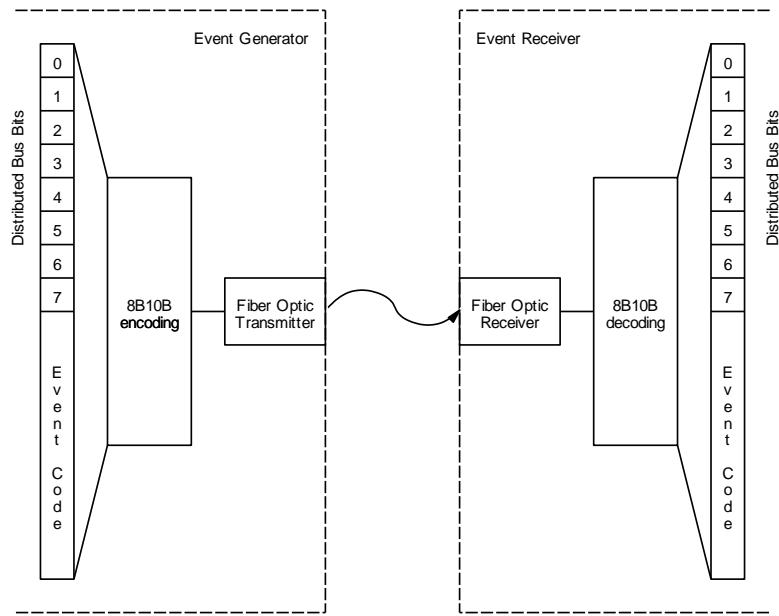


Figure 1: Event Frame

## Event Codes

There are 256 event codes from which a few have special functions. The special function event codes are listed below. Only one event code may be transferred at a time. If there is no event code to be transferred, the null event code (0x00) is transmitted. Every now and then a special 8B10B character K28.5 is transmitted instead of the null event code. The K28.5 comma character is

transmitted to allow the event receivers to synchronise on the correct word boundary is the serial bit stream.

Event Code	Code Name	EVG Function	EVRI Function
0x00	Null Event Code	-	-
0x01 – 0x6F	-	User Defined	User Defined
0x70	Seconds '0'	-	Shift in '0' to LSB of Seconds Shift Register
0x71	Seconds '1'	-	Shift in '1' to LSB of Seconds Shift Register
0x72 – 0x79	-	User Defined	User Defined
0x7A	Heartbeat	-	Reset Heartbeat Monitor
0x7B	Synchronise Prescalers	-	Synchronise Prescaler Outputs
0x7C	Timestamp Counter Increment	-	Increment Timestamp Counter
0x7D	Timestamp Counter Reset	-	Reset Timestamp Counter
0x7F	End of Sequence	Stop Sequence	-
0x80-FF	-	User Defined	User Defined

## Distributed Bus and Data Transmission


The distributed bus allows transmission of eight simultaneous signals with the event clock rate time resolution (10 ns at 100 MHz event clock rate). The source for distributed bus signals may come from an external source or the signals may be generated with programmable multiplexed counters (MXC) inside the event generator. The distributed bus signals may be programmed to be available as hardware outputs on the event receiver.

In latest firmware versions the distributed bus bandwidth may be shared by transmission of a configurable size data buffer to up to 2 kbytes. When data transmission is enabled the distributed bus bandwidth is halved. The remaining bandwidth is reserved for transmitting data with a speed up to 50 Mbytes/s (event clock rate divided by two).

## Event Sources

### Trigger Events

There are eight trigger event sources that send out an event code on a stimulus. Each trigger event has its own programmable event code register and various enable bits. The event code transmitted is determined by contents of the corresponding event code register. The stimulus may be a detected rising edge on an external signal or a rising edge of a multiplexed counter output.

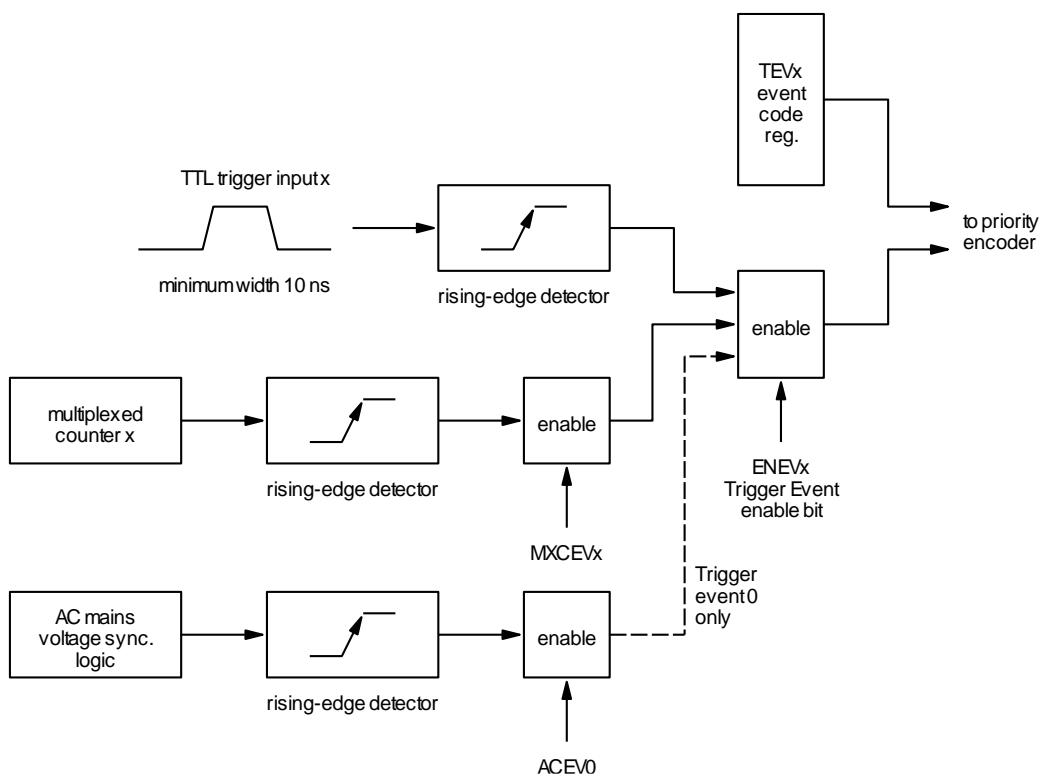

**Figure 2: Trigger Events**

Trigger Event 0 has also the option of being triggered by a rising edge of the AC mains voltage synchronization logic output signal.

The external input accepts TTL level signals. The input logic is edge sensitive and the signals are synchronized internally to the event clock.

## Upstream Events

Event Generators may be cascaded. The event generator receiver includes a first-in-first-out (FIFO) memory to synchronize incoming events which may be synchronized to a clock unrelated to the event clock. Usually there are no events in the FIFO. An event code from an upstream EVG is transmitted as soon as there is no other event code to be transmitted.

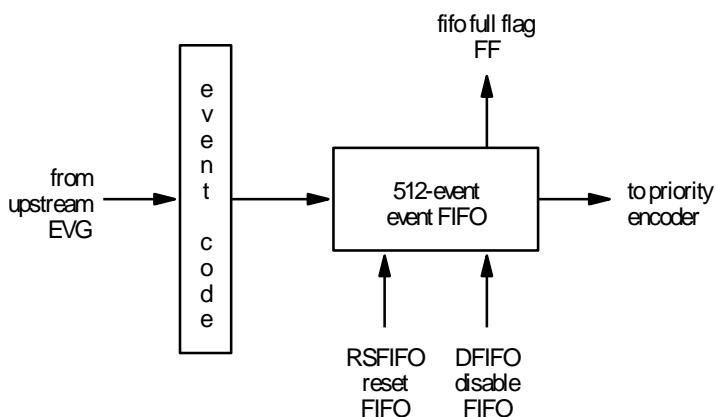


Figure 3: Upstream Event FIFO

## Event Sequencer

Event sequencers provide a method of transmitting or playing back sequences of events stored in random access memory with defined timing. In the event generator there are two event sequencers. The 8-bit event codes are stored in a RAM table each attached with a 32-bit timestamp relative to the start of sequence. Both sequencers can hold up to 2048 event code – timestamp pairs.

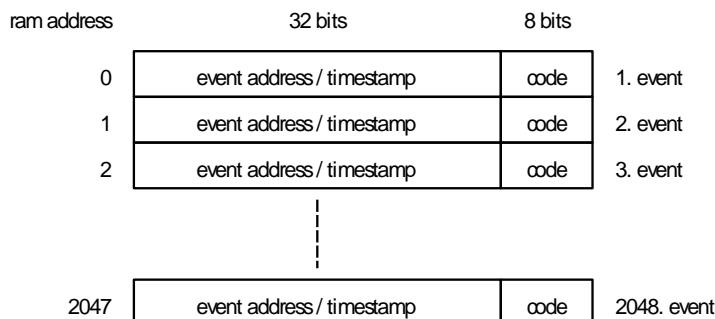


Figure 4: Sequencer RAM Structure

The contents of a sequencer RAM may be altered at any time, however, it is recommended only to modify RAM contents when the RAM is disabled. The sequencer runs at the event clock rate to up to 100 MHz.

The Sequencers may be triggered from several sources including software triggering, triggering on a multiplexed counter output or AC mains voltage synchronization logic output.

The sequencers are enabled by writing a '1' bit to SQxEN in the Sequence RAM control Register. The RAMs may be disabled any time by writing a '1' to SQxDIS bit. Disabling sequence RAMs does not reset the RAM address and timestamp registers. By writing a '1' to the bit SQxRES in the Control Register the sequencer is both disabled and the RAM address and timestamp register is reset.

When the sequencer is triggered the internal event address counters starts counting. The counter value is compared to the event address of the next event in the RAM table. When the counter value matches or is greater than the timestamp in the RAM table, the attached event code is

transmitted. The time offset between two consecutive events in the RAM is allowed to be 1 to  $2^{32}$  sequence clock cycles i.e. the internal event address counter rolls over when to 0 when 0xffffffff is reached.

There are two special event codes which are not transmitted, the null event code 0x00 and end sequence code 0x7f. The null event code may be used if the time between two consecutive events should exceed  $2^{32}$  event clock cycles by inserting a null event with a timestamp value of 0xffffffff. The end sequence code resets the sequencer RAM table address and timestamp register and depending on configuration bits, disables the sequencer (single sequence, SQxSNG=1) or restarts the sequence either immediately (recycle sequence, SQxREC=1) or waits for a new trigger (SQxREC=0).

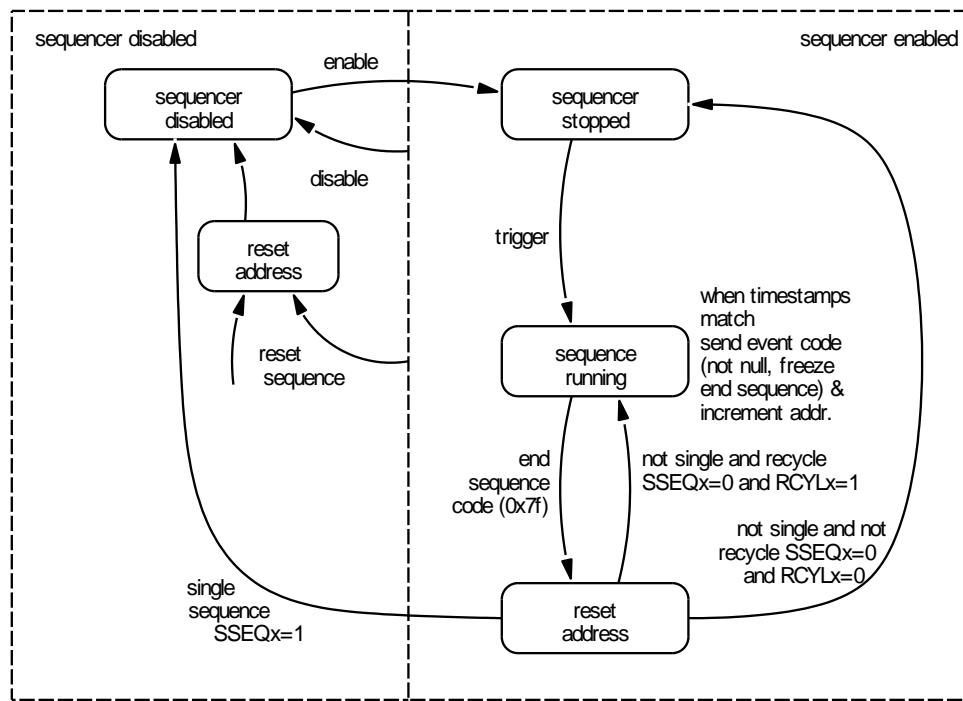


Figure 5: Sequencer Control


## Sequencer Interrupt Support

The sequencers provide two interrupts: a sequence start and sequence stop interrupt. The sequence start interrupt is issued when a sequencer is in enabled state, gets triggered and was not running before the trigger.

A sequence stop interrupt is issued when the sequence is running and reaches the 'end of sequence' code.

## Distributed Bus


The bits of the distributed bus are sampled at the event rate from external signals; alternatively the distributed bus signals may be generated by multiplexed counter outputs. If there is an upstream EVG, the state of all distributed bus bits may be forwarded by the EVG.

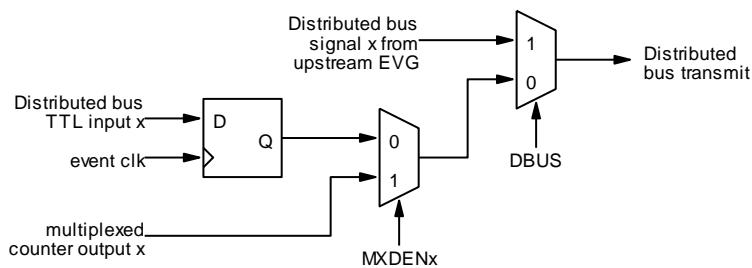

**Figure 6: Distributed Bus**

## Timestamping Inputs

Starting from firmware version E306 a few distributed bus input signals have dual function: transition board input DBUS5-7 can be used to generate special event codes controlling the timestamping in Event Receivers.

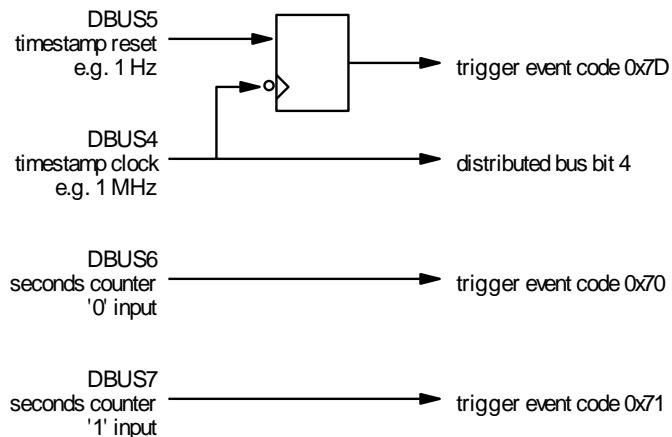

**Figure 7: Timestamping Inputs**

The two clocks, timestamp clock and timestamp reset clock, are assumed to be rising edge aligned. In the EVG the timestamp reset clock is sampled with the falling edge of the timestamp clock. This is to prevent a race condition between the reset and clock signals. In the EVR the reset is synchronised with the timestamp clock.

The two seconds counter events are used to shift in a 32-bit seconds value between consecutive timestamp reset events. In the EVR the value of the seconds shift register is transferred to the seconds counter at the same time the higher running part of the timestamp counter is reset.

The distributed bus event inputs can be enabled independently through the distributed bus event enable register. The events generated through these distributed bus input ports are given lowest priority.

## Timestamp Generator

Logic has been added to automatically increment and send out the 32-bit seconds value. Using this feature requires the two externally supplied clocks as shown above, but the events 0x70 and 0x71 get generated automatically.

After the rising edge of the slower clock on DBUS4, the internal seconds counter is incremented and the 32 bit binary value is sent out LSB first as 32 events 0x70 and 0x71. The seconds counter can be updated by software by using the TSValue and TSControl registers.

## Multiplexed Counters

Eight 32-bit multiplexed counters generate clock signals with programmable frequencies from event clock/ $2^{32}-1$  to event clock/2. Even divisors create 50% duty cycle signals. The counter outputs may be programmed to trigger events, drive distributed bus signals and trigger sequence RAMs. The output of multiplexed counter 7 is hard-wired to the mains voltage synchronization logic.

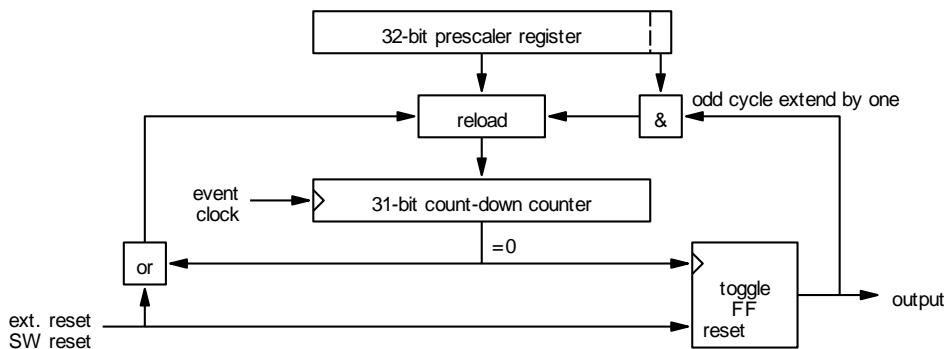


Figure 8: Multiplexed Counter


Each multiplexed counter consists of a 32-bit prescaler register and a 31-bit count-down counter which runs at the event clock rate. When count reaches zero, the output of a toggle flip-flop changes and the counter is reloaded from the prescaler register. If the least significant bit of the prescaler register is one, all odd cycles are extended by one clock cycle to support odd dividers.

Prescaler value	Duty Cycle	Frequency at 125 MHz Event Clock
0, 1 not allowed	undefined	Undefined
2	50/50	62.5 MHz
3	33/66	41.7 MHz
4	50/50	31.25 MHz
5	40/60	25 MHz
...	...	...
$2^{32}-1$	approx. 50/50	0.029 Hz

The multiplexed counters may be reset by software or hardware input. The reset state is defined by the multiplexed counter polarity register.

## Configurable Size Data Buffer

Starting from firmware version E305 transmission of a configurable size data buffer over the event system link is possible. The buffer size can be programmed in four byte increments (long words) from 4 bytes to 2048 bytes.

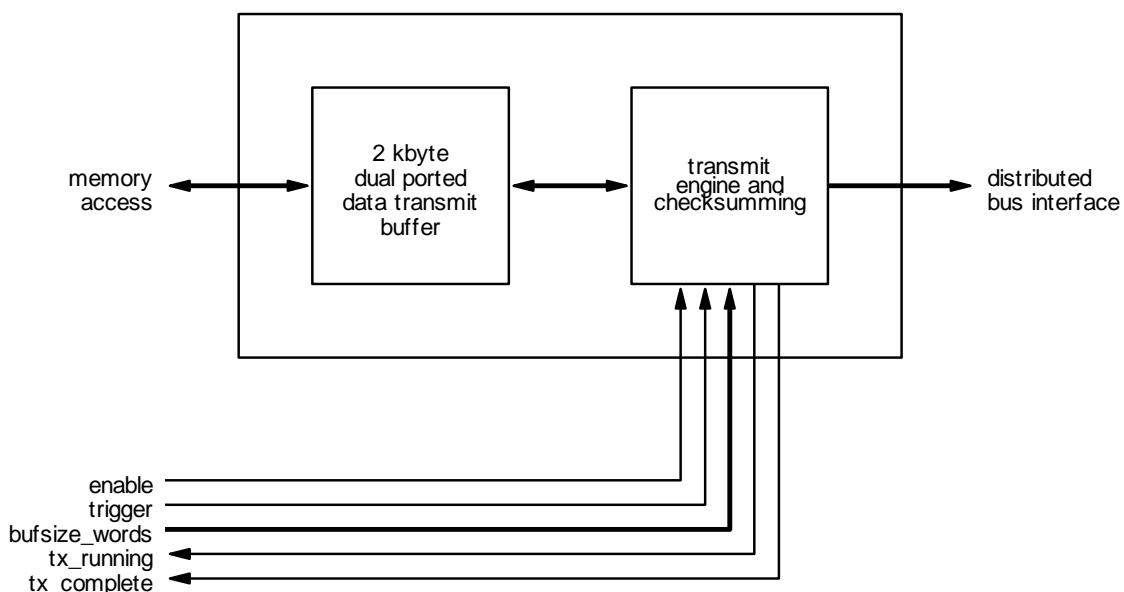

**Figure 9: Configurable size transmit data buffer**

When the EVG is configured for data transmission (*mode* = 1 in data buffer control register) the bandwidth of the distributed bus is shared with data transmission: half of the bandwidth remains for the distributed bus and the other half is reserved for data transmission.

The data to be transmitted is stored in a 2 kbyte dual-ported memory starting from the lowest address 0. This memory is directly accessible from VME. The transfer size is determined by *bufsize* register bits in four byte increments. The transmission is trigger by software. Two flags *tx\_running* and *tx\_complete* represent the status of transmission.

Transmission utilises two K-characters to mark the start and end of the data transfer payload, the protocol looks following:

**Table 1: Data Transmission Protocol**

<b>8B10B-character</b>	<b>Description</b>
K28.0	Start of data transfer
Dxx.x	1 <sup>st</sup> data byte (address 0)
Dxx.x	2 <sup>nd</sup> data byte (address 1)
Dxx.x	3 <sup>rd</sup> data byte (address 2)
Dxx.x	4 <sup>th</sup> data byte (address 3)
...	...
Dxx.x	n <sup>th</sup> data byte (address n-1)
K28.1	End of data
Dxx.x	Checksum (LSB)
Dxx.x	Checksum(MSB)

## Programmable Front Panel Connections


The front panel outputs are programmable: multiplexed counters and distributed bus bits can be mapped to any output. The mapping is shown in table below.

**Table 2: Signal mapping IDs**

Mapping ID	Signal
0 to 31	(Reserved)
32	Distributed bus bit 0 (DBUS0)
...	...
39	Distributed bus bit 7 (DBUS7)
40	Multiplexed Counter 0
...	...
47	Multiplexed Counter 7
48 to 61	(Reserved)
62	Force output high (logic 1)
63	Force output low (logic 0)

## AC Line Synchronisation

The Event Generator provides synchronization to the mains voltage frequency or another external clock. The mains voltage frequency can be divided by an eight bit programmable divider. The output of the divider may be delayed by 0 to 25.5 ms by a phase shifter in 0.1 ms steps to be able to adjust the triggering position relative to mains voltage phase. After this the signal synchronized to the event clock or the output of multiplexed counter 7.

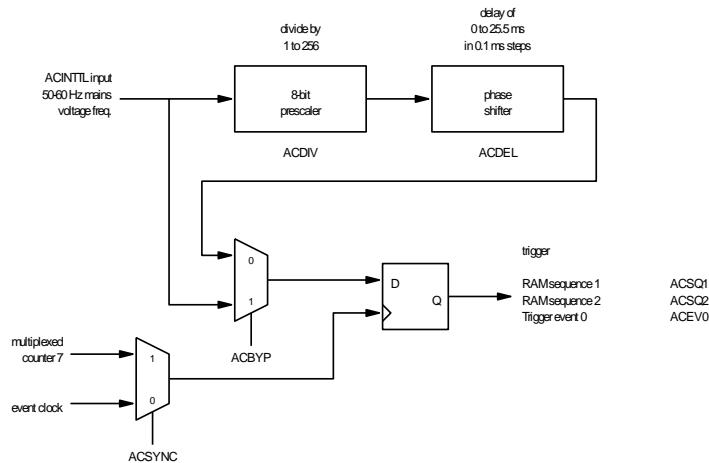

**Figure 10: AC Input**

The phase shifter operates with a clock of 1 MHz which introduces jitter. If the prescaler and phase shifter are not required this circuit may be bypassed. This also reduces jitter because the external trigger input is sampled directly with the event clock.

## Event Clock

All operations on the event generator are synchronised to the event clock which is derived from an externally provided RF clock. For laboratory testing purposes an on-board fractional

synthesiser may be used to deliver the event clock. The serial link bit rate is 20 times the event clock rate. The acceptable range for the event clock and bit rate is shown in the following table.

	Event Clock	Bit Rate
Minimum	50 MHz	1.0 Gb/s
Maximum	125 MHz	2.5 Gb/s

Note: maximum event clock for cPCI-EVG-220 is 100 MHz with 2.0 Gb/s bit rate

During operation the reference frequency should not be changed more than  $\pm 100$  ppm.

## **RF Clock and Event Clock**

The event clock may be derived from an external RF clock signal. The front panel RF input is 50 ohm terminated and AC coupled to a LVPECL logic input, so either an ECL level clock signal or sine-wave signal with a level of maximum +10 dBm can be used.

Divider	RF Input Frequency	Event Clock	Bit Rate
$\div 1$	50 MHz – 125 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 2$	100 MHz – 250 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 3$	150 MHz – 375 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 4$	200 MHz – 500 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 5$	250 MHz – 625 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 6$	300 MHz – 750 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 7$	350 MHz – 875 MHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 8$	400 MHz – 1.0 GHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 9$	450 MHz – 1.125 GHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 10$	500 MHz – 1.25 GHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 11$	550 MHz – 1.375 GHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 12$	600 MHz – 1.5 GHz	50 MHz – 125 MHz	1.0 Gb/s – 2.5 Gb/s
$\div 14$	700 MHz – 1.6 GHz *)	50 MHz – 114 MHz	1.0 Gb/s – 2.286 Gb/s
$\div 15$	750 MHz – 1.6 GHz *)	50 MHz – 107 MHz	1.0 Gb/s – 2.133 Gb/s
$\div 16$	800 MHz – 1.6 GHz *)	50 MHz – 100 MHz	1.0 Gb/s – 2.0 Gb/s
$\div 17$	850 MHz – 1.6 GHz *)	50 MHz – 94 MHz	1.0 Gb/s – 1.882 Gb/s
$\div 18$	900 MHz – 1.6 GHz *)	50 MHz – 88 MHz	1.0 Gb/s – 1.777 Gb/s
$\div 19$	950 MHz – 1.6 GHz *)	50 MHz – 84 MHz	1.0 Gb/s – 1.684 Gb/s
$\div 20$	1.0 GHz – 1.6 GHz *)	50 MHz – 80 MHz	1.0 Gb/s – 1.600 Gb/s
$\div 21$	1.05 GHz – 1.6 GHz *)	50 MHz – 76 MHz	1.0 Gb/s – 1.523 Gb/s
$\div 22$	1.1 GHz – 1.6 GHz *)	50 MHz – 72 MHz	1.0 Gb/s – 1.454 Gb/s
$\div 23$	1.15 GHz – 1.6 GHz *)	50 MHz – 69 MHz	1.0 Gb/s – 1.391 Gb/s
$\div 24$	1.2 GHz – 1.6 GHz *)	50 MHz – 66 MHz	1.0 Gb/s – 1.333 Gb/s
$\div 25$	1.25 GHz – 1.6 GHz *)	50 MHz – 64 MHz	1.0 Gb/s – 1.280 Gb/s
$\div 26$	1.3 GHz – 1.6 GHz *)	50 MHz – 61 MHz	1.0 Gb/s – 1.230 Gb/s
$\div 27$	1.35 GHz – 1.6 GHz *)	50 MHz – 59 MHz	1.0 Gb/s – 1.185 Gb/s
$\div 28$	1.4 GHz – 1.6 GHz *)	50 MHz – 57 MHz	1.0 Gb/s – 1.142 Gb/s
$\div 29$	1.45 GHz – 1.6 GHz *)	50 MHz – 55 MHz	1.0 Gb/s – 1.103 Gb/s
$\div 30$	1.5 GHz – 1.6 GHz *)	50 MHz – 53 MHz	1.0 Gb/s – 1.066 Gb/s
$\div 31$	1.55 GHz – 1.6 GHz *)	50 MHz – 51 MHz	1.0 Gb/s – 1.032 Gb/s
$\div 32$	1.6 GHz *)	50 MHz	1.0 Gb/s

\*) Range limited by AD9515 maximum input frequency of 1.6 GHz

Note: maximum event clock for cPCI-EVG-220 is 100 MHz with 2.0 Gb/s bit rate

## Fractional Synthesiser

For laboratory testing purposes the event clock may be generated on-board the event generator using a fractional synthesiser. A Micrel (<http://www.micrel.com>) SY87739L Protocol Transparent Fractional-N Synthesiser with a reference clock of 24 MHz is used. The following table lists programming bit patterns for a few frequencies.

Event Rate	Configuration Bit Pattern	Reference Output	Precision (theoretical)
499.8 MHz/4 = 124.95 MHz	0x00FE816D	124.95 MHz	0
499.654 MHz/4 = 124.9135 MHz	0x0C928166	124.907 MHz	-52 ppm
476 MHz/4 = 119 MHz	0x018741AD	119 MHz	0
106.25 MHz (fibre channel)	0x049E81AD	106.25 MHz	0
499.8 MHz/5 = 99.96 MHz	0x025B41ED	99.956 MHz	-40 ppm
50 MHz	0x009743AD	50.0 MHz	0
499.8 MHz/10 = 49.98 MHz	0x025B43AD	49.978 MHz	-40 ppm
499.654 MHz/4 = 124.9135 MHz	0x0C928166	124.907 MHz	-52 ppm
50 MHz	0x009743AD	50.0 MHz	0

## Connections

### cPCI-EVG-2x0 Front Panel Connections

The front panel of the Event Generator and its optional side-by-side module is shown in Figure 11 and Figure 12.

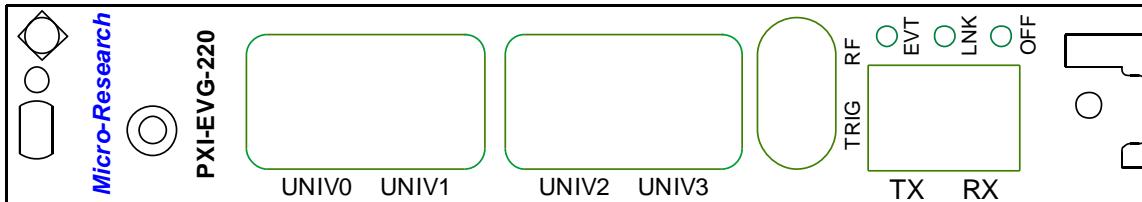


Figure 11: Event Generator Front Panel

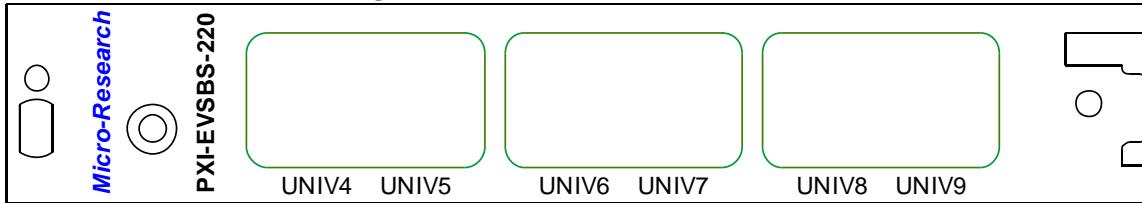


Figure 12: Optional Side-by-side Module Front Panel

The front panel of the Event Generator includes the following connections and status leds:

Connector / Led	Style	Level	Description
LNK	Red/Green Led		Red: receiver violation detected Green: RX link OK, violation flag cleared
EVT	Red/Green Led		Green: link OK, flashes when event code received Red: Flashes on led event
TX	LC	optical	Transmit Optical Output (TX)
RX	LC	optical	Receiver Optical Input (RX)
RF	LEMO-EPY	RF	RF/event clock input
TRIG	LEMO-EPY	TTL	AC Trigger input
UNIV0/1	Universal slot		Universal Input 0/1
UNIV2/3	Universal slot		Universal Input 2/3
UNIV4/5	Universal slot		Universal Input 4/5
UNIV6/5	Universal slot		Universal Input 6/7
UNIV8/9	Universal slot		Universal Input 8/9

## VME-EVG-230 Front Panel Connections

The front panel of the Event Generator is shown in Figure 11.




Figure 13: Event Generator Front Panel

The front panel of the Event Generator includes the following connections and status LEDs:

Connector / Led	Style	Level	Description
FAIL	Red Led		Module Failure
OFF	Blue Led		Module Powered Down
RX LINK	Green Led		Receiver Link Signal OK
ENA	Green Led		Event Generator Enabled
EVENT IN	Yellow Led		Incoming Event (RX)
EVENT OUT	Yellow Led		Outgoing Event (TX)
RX FAIL	Red Led		Receiver Violation
ERR	Red Led		SY87739L reference not locked
RUN	Green Led		Ubicom IP2022 Running
ACT	Yellow Led		Ubicom IP2022 Telnet connection active
10baseT	RJ45	10baseT	Ubicom 10baseT Ethernet Connection with link (green) and active (amber) leds
10/100	RJ45		(reserved)
TX	LC	optical	Transmit Optical Output (TX)
RX	LC	optical	Receiver Optical Input (RX)
ACIN	LEMO-EPY	TTL	Trigger input
RFIN	LEMO-EPY	RF +10 dBm	RF Reference Input
IN0	LEMO-EPY	TTL	Configurable front panel input
IN1	LEMO-EPY	TTL	Configurable front panel input
OUT0	LEMO-EPY	TTL	Configurable front panel output
OUT1	LEMO-EPY	TTL	Configurable front panel output
OUT2	LEMO-EPY	TTL	Configurable front panel output
OUT3	LEMO-EPY	TTL	Configurable front panel output
OUT4	LEMO-EPY	TTL	Configurable front panel output
OUT5	LEMO-EPY	TTL	Configurable front panel output
UNIV0	Universal I/O		Configurable Universal I/O input
UNIV1	Universal I/O		Configurable Universal I/O input
UNIV2	Universal I/O		Configurable Universal I/O input
UNIV3	Universal I/O		Configurable Universal I/O input
COM	RJ45	RS232	Reserved

## VME-EVG-230 VME P2 User I/O Pin Configuration

The following table lists the connections to the VME P2 User I/O Pins.

<b>Pin</b>	<b>Signal</b>
A1	Transition board ID0
A2	Transition board ID1
A3-A10	Ground
A11	Transition board ID2
A12	Transition board ID3
A13-A15	Ground
A16	Transition board handle switch
A17-A26	Ground
A27-A31	+5V
A32	Power control for transition board
C1	Transition board input 0
C2	Transition board input 1
C3	Transition board input 2
C4	Transition board input 3
C5	Transition board input 4
C6	Transition board input 5
C7	Transition board input 6
C8	Transition board input 7
C9	Transition board input 8
C10	Transition board input 9
C11	Transition board input 10
C12 – C27	(reserved input)
C28	Transition board input 11
C29	Transition board input 12
C30	Transition board input 13
C31	Transition board input 14
C32	Transition board input 15

## cPCI-EVG-300 Front Panel Connections




Figure 14: cPCI-EVG-300 Event Receiver Front Panel

Connector / Led	Style	Level	Description
UNIV0/1	Universal slot		Universal Output 0/1
UNIV2/3	Universal slot		Universal Output 2/3
UNIV4/5	Universal slot		Universal Output 4/5
UNIV6/7	Universal slot		Universal Output 6/7

UNIV8/9	Universal slot		Universal Output 8/9
UNIV10/11	Universal slot		Universal Output 10/11
USB	USB		(USB Serial Port, reserved)
10/100	RJ45		(10/100 Ethernet, reserved)
TRIG	Lemo	TTL	TTL AC Trigger Input
RF	Lemo	RF +10 dBm	RF Reference Input
Link TX (SFP)	LC	Optical 850 nm	Event link Transmit
Link RX (SFP)	LC	Optical 850 nm	Event link Receiver

### **PXIe-EVG-300 Front Panel Connections**

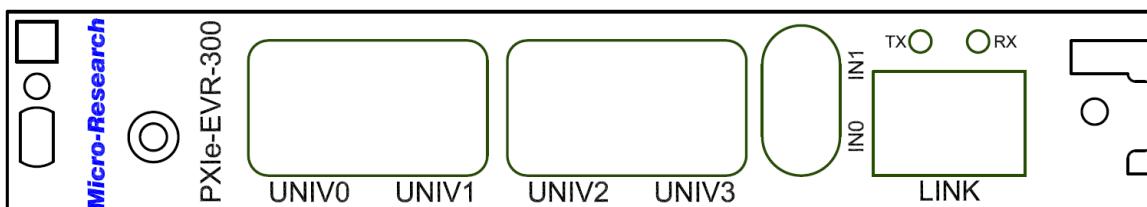


Figure 15: PXIe-EVG-300 Event Receiver Front Panel

The front panel of the Event Receiver includes the following connections and status leds:

Connector / Led	Style	Level	Description
RX led	RGB Led		Red: receiver violation detected Green: RX link OK, violation flag cleared Yellow: RX link OK, violation detected
TX led	RGB Led		Green: link OK, flashes when event code received Red: Flashes on led event
LINK TX	LC	optical	Transmit Optical Output (TX)
LINK RX	LC	optical	Receiver Optical Input (RX)
RF	LEMO-EPY	RF	RF/event clock input
TRIG	LEMO-EPY	TTL	AC Trigger input
UNIV0/1	Universal slot		Universal Output 0/1
UNIV2/3	Universal slot		Universal Output 2/3

### **PXIe-EVG-300 Backplane Connections**

The PXIe-EVG-300 provides a number of backplane I/O signals, conventional PXI timing and synchronization signals and new differential signals introduced by the PXI Express specification.

The PXI trigger bus and the the PXI star triggers are bidirectional. The direction of the signal path is specified by the output mapping register: the output has to be tri-stated for an external device to drive the signal.

PXIe Signal	EVG Input Signal	EVG Output Signal	Description
PXI_TRIGGER[0:7]	TBIN[0:7]	TBOUT[0:7]	PXI trigger bus

PXI_STAR[0:16]	TBIN[8:24]	TBOUT[8:24]	PXI star triggers
PXIe_DSTARA[0:16]	n/a	TBOUT[25:41]	PXIe differential LVPECL star triggers
PXIe_DSTARB[0:16]	n/a	TBOUT[42:58]	PXIe differential LVDS star triggers
PXIe_DSTARC[0:16]	TBIN[25:41]	n/a	PXIe differential LVDS star input signals

## Programming Details

### **VME-EVG-230 CR/CSR Support**

The VME Event Generator module provides CR/CSR Support as specified in the VME64x specification. The CR/CSR Base Address Register is determined after reset by the inverted state of VME64x P1 connector signal pins GA4\*-GA0\*. In case the parity signal GAP\* does not match the GAx\* pins the CR/CSR Base Address Register is loaded with the value 0xf8 which corresponds to slot number 31.

Note: the board can be used in standard VME crates where geographical pins do not exist, in this case the user may either insert jumpers to set the geographical address or use the default setting when the board's CR/CSR base address will be set to 0xf8.

After power up or reset the board responds only to CR/CSR accesses with its geographical address. Prior to accessing Event Generator functions the board has to be configured by accessing the boards CSR space.

The Configuration ROM (CR) contains information about manufacturer, board ID etc. to identify boards plugged in different VME slots. The following table lists the required field to locate an Event Generator module.

CR address	Register	EVG
0x27, 0x2B, 0x2F	Manufacturer's ID (IEEE OUI)	0x000EB2
0x33, 0x37, 0x3B, 0x3F	Board ID	0x454700E6

For convenience functions are provided to locate VME64x capable boards in the VME crate.

```
STATUS vmeCRFindBoard(int slot, UINT32 ieee_oui, UINT32 board_id,  
                      int *p_slot);
```

To locate the first Event Generator in the crate starting from slot 1, the function has to be called following:

```
#include "vme64x_cr.h"  
int slot = 1;  
int slot_evg;  
vmeCRFindBoard(slot, 0x000EB2, 0x454700E6, &slot_evg);  
or  
vmeCRFindBoard(slot, MRF_IEEE_OUI, MRF_4CHTIM_BID, &slot_evg);
```

If this function returns OK, an Event Generator board was found in slot slot\_evg.

### **Function 0/1/2 Registers**

The Event Generator specific register are accessed via Function 0, 1 or 2 as specified in the VME64x specification. To enable Function 0, the address decoder compare register for Function 0 in CSR space has to be programmed. For convenience a function to perform this is provided:

```
STATUS vmeCSRWriteADER(int slot, int func, UINT32 ader);
```

To configure Function 0 of an Event Generator board in slot 3 to respond to A16 accesses at the address range 0x1800-0x1FFF the function has to be called with following values:

```
vmeCSRWriteADER(3, 0, 0x18A4);
```

ADER contents are composed of the address mask and address modifier, the above is the same as:

```
vmeCSRWriteADER(3, 0, (slot << 11) | (VME_AM_SUP_SHORT_IO << 2));
```

To get the memory mapped pointer to the configured Function 0 registers on the Event Generator board the following VxWorks function has to be called:

```
MrfEvgStruct *pEvg;  
sysBusToLocalAdrs(VME_AM_SUP_SHORT_IO, (char *) (slot << 11),  
                   (void *) pEvg);
```

**Note:** using the data transmission capability requires reserving more than 4 kbytes for function 0 i.e. use of addressing mode A24 is suggested, following:

```
vmeCSRWriteADER(3, 0, (slot << 19) | (VME_AM_STD_USR_DATA << 2));  
MrfEvgStruct *pEvg;  
sysBusToLocalAdrs(VME_AM_STD_USR_DATA, (char *) (slot << 19),  
                   (void *) pEvg);
```

## VME-EVG-230 Network Interface

A 10baseT network interface is provided to upgrade the FPGA firmware and set up boot options. It is also possible to control the module over the network interface.

### **Assigning an IP Address to the Module**

By default the modules uses DHCP (dynamic host configuration protocol) to acquire an IP address. In case a lease cannot be acquired the IP address set randomly in the 169.254.x.x subnet. The board can be programmed to use a static address instead if DHCP is not available.

The module can be located looking at the lease log of the DHCP server or using a Windows tool called Locator.exe.

### **Using Telnet to Configure Module**

To connect to the configuration utility of the module issue the following command:

```
telnet 192.168.1.32 23
```

The latter parameter is the telnet port number and is required in Linux to prevent negotiation of telnet parameters which the telnet server of the module is not capable of.

The telnet server responds to the following commands:

Command	Description
b	Show/change boot parameters, IP address etc.
d	Dump 16 bytes of memory
h / ?	Show Help
i	Read & show dynamic configuration values from FPGA
m <address> [<data>]	Read/Write FPGA CR/CSR, Function 0
r	Reset Board
s	Save boot configuration & dynamic configuration values into non-volatile memory
u	Update IP2022 software
q	Quit Telnet

### **Boot Configuration (command b)**

Command b displays the current boot configuration parameters of the module. The parameter may be changed by giving a new parameter value. The following parameters are displayed:

Parameter	Description
Use DHCP	0 = use static IP address, 1 = use DHCP to acquire address, net mask etc.
IP address	IP address of module
Subnet mask	Subnet mask of module
Default GW	Default gateway
FPGA mode	FPGA configuration mode 0 – FPGA is not configured after power up

	1 – FPGA configured from internal Flash memory 2 – FPGA is configured from FTP server
FTP server	FTP server IP address where configuration bit file resides
Username	FTP server username
Password	FTP server password
FTP Filename	FTP server configuration file name
Flash Filename	Configuration file name on internal flash
μs divider	Integer divider to get from event clock to 1MHz, e.g. 125 for 124.9135 MHz
Fractional divider configuration word	Micrel SY87739UMI fractional divider configuration word to set reference for event clock

Note that after changing parameters the parameters have to be saved to internal flash by issuing the Save boot configuration (s) command. The changes are applied only after resetting the module using the reset command or hardware reset/power sequencing.

### Memory dump (command d)

This command dumps 16 bytes of memory starting at the given address, if the address is omitted the previous address value is increased by 16 bytes.

The most significant byte of the address determines the function of the access:

Address	Function
0x00000000	CR/CSR space access
0x80000000	EVG registers access

To dump the start of the EVG register map issue the 'd' command from the telnet prompt:

```
VME-EVG-230 -> d 80000000 ↵
Addr 80000000: d000 0001 0000 0000 0000 0000 0000 0000
VME-EVG-230 -> d ↵
Addr 80000010: 0000 0000 0000 0000 0000 0000 0000 0000
VME-EVG-230 ->
```

### Memory modify (commands d and m)

The access size is always a short word i.e. two bytes.

To check the status register from the telnet prompt:

```
VME-EVG-230 -> m 80000000 ↵
Addr 80000000 data d000
VME-EVG-230 ->
```

To enable the EVG issue:

```
VME-EVG-230 -> m 80000000 0000 ↵
Addr 80000000 data 4001
VME-EVG-230 ->
```

## Upgrading IP2022 Microprocessor Software (command u)

To upgrade the Ubicom IP2022 microprocessor software download the upgrade image containing the upgrade to the module using TFTP:

### Linux

In Linux use e.g. interactive tftp:

```
$ tftp 192.168.1.32
tftp> bin
tftp> put upgrade.bin /fw
tftp> quit
```

### Windows

In Windows command prompt issue the following command:

```
C:\> tftp -i 192.168.1.32 PUT upgrade.bin /fw
```

When the upgrade image has been downloaded and verified, enter at the telnet prompt following:

```
VME-EVG-230 -> u ↵
Really update firmware (yes/no) ? yes ↵
Self programming triggered.
```

The Event Generator starts programming the new software and restarts.

## Upgrading FPGA Configuration File

When the FPGA configuration file resides in internal flash memory a new file system image has to be downloaded to the module. This is done using TFTP protocol:

### Linux

In Linux use e.g. interactive tftp:

```
$ tftp 192.168.1.32
tftp> bin
tftp> put filesystem.bin /
tftp> quit
```

### Windows

In Windows command prompt issue the following command:

```
C:\> tftp -i 192.168.1.32 PUT filesystem.bin /
```

Now the FPGA configuration file has been upgraded and the new configuration is loaded after next reset/power sequencing.

**Note!** Due to the UDP protocol it is recommended to verify (read back and compare) the filesystem image before restarting the module. This is done following:

## Linux

In Linux use e.g. interactive tftp:

```
$ tftp 192.168.1.32
tftp> bin
tftp> get / verify.bin
tftp> quit
$ diff filesystem.bin verify.bin
$
```

If files differ you should get following message:

Binary files filesystem.bin and verify.bin differ

## Windows

In Windows command prompt issue the following command:

```
C:\> tftp -i 192.168.1.32 GET / verify.bin
C:\> fc /b filesystem.bin verify.bin
Comparing files filesystem.bin and verify.bin
FC: no differences encountered
```

## **UDP Remote Programming Protocol**

The VME-EVG can be remotely programmed using the 10baseT Ethernet interface with a protocol over UDP (User Datagram Protocol) which runs on top of IP (Internet Protocol). The default port for remote programming is UDP port 2000. The UDP commands are built upon the following structure:

access_type (1 byte)	status (1 byte)	data (2 bytes)
	address (4 bytes)	
	ref (4 bytes)	

The first field defines the access type:

access_type	Description
0x01	Read Register from module
0x02	Write and Read back Register from module

The second field tells the status of the access:

Status	Description
0	Command OK
-1	Bus ERROR (Invalid read/write address)
-2	Timeout (FPGA did not respond)
-3	Invalid command

The access size is always a short word i.e. two bytes. The most significant byte of the address determines the function of the access:

Address	Function

0x00000000	CR/CSR space access
0x80000000	EVG registers access

**Read Access (Type 0x01)**

The host sends a UDP packet to port 2000 of the VME-EVG with the following contents:

access_type (1 byte) 0x01	status (1 byte) 0x00	data (2 bytes) 0x0000
address (4 bytes) 0x80000000 (Control and Status register Function 0 address)		
ref (4 bytes) 0x00000000		

If the read access is successful the VME-EVG replies to the same host and port the message came from with the following packet:

access_type (1 byte) 0x01	status (1 byte) 0x00	data (2 bytes) 0xD000
address (4 bytes) 0x80000000 (Control and Status register Function 0 address)		
ref (4 bytes) 0x00000000		

**Write Access (Type 0x02)**

The host sends a UDP packet to port 2000 of the VME-EVG with the following contents:

access_type (1 byte) 0x02	status (1 byte) 0x00	data (2 bytes) 0x0001
Address (4 bytes) 0x80000002 (Event enable register Function 0 address)		
ref (4 bytes) 0x00000000		

If the write access is successful the VME-EVG replies to the same host and port the message came from with the following packet:

access_type (1 byte) 0x02	status (1 byte) 0x00	data (2 bytes) 0x0001
address (4 bytes) 0x80000002 (Event enable register Function 0 address)		
ref (4 bytes) 0x00000000		

Notice that in the reply message the data returned really is the data read from the address specified in the address field so one can verify that the data really was written ok.

**Register Map**

Address	Register	Type	Description
0x000	Status	UINT32	Status Register
0x004	Control	UINT32	Control Register
0x008	IrqFlag	UINT32	Interrupt Flag Register
0x00C	IrqEnable	UINT32	Interrupt Enable Register
0x010	ACControl	UINT32	AC divider control
0x014	ACMap	UINT32	AC trigger event mapping
0x018	SWEvent	UINT32	Software event register
0x020	DataBufControl	UINT32	Data Buffer Control Register
0x024	DBusMap	UINT32	Distributed Bus Mapping Register
0x028	DBusEvents	UINT32	Distributed Bus Timestamping Events Register
0x02C	FWVersion	UINT32	Firmware Version Register
0x034	TSCControl	UINT32	Timestamp event generator control register
0x038	TSValue	UINT32	Timestamp event generator value register
0x04C	UseC Divider	UINT32	Divider to get from Event Clock to 1 MHz
0x050	ClockControl	UINT32	Event Clock Control Register
0x060	EvanControl	UINT32	Event Analyser Control Register
0x064	EvanCode	UINT32	Event Analyser Distributed Bus and Event Code Register
0x068	EvanTimeHigh	UINT32	Event Analyser Time Counter (bits 63 – 32)
0x06C	EvanTimeLow	UINT32	Event Analyser Time Counter (bits 31 – 0)
0x070	SeqRamCtrl0	UINT32	Sequence RAM 0 Control Register
0x074	SeqRamCtrl1	UINT32	Sequence RAM 1 Control Register
0x080	FracDiv	UINT32	Micrel SY87739L Fractional Divider Configuration Word
0x100	EvTrig0	UINT32	Event Trigger 0 Register
0x104	EvTrig1	UINT32	Event Trigger 1 Register
0x108	EvTrig2	UINT32	Event Trigger 2 Register
0x10C	EvTrig3	UINT32	Event Trigger 3 Register
0x110	EvTrig4	UINT32	Event Trigger 4 Register
0x114	EvTrig5	UINT32	Event Trigger 5 Register
0x118	EvTrig6	UINT32	Event Trigger 6 Register
0x11C	EvTrig7	UINT32	Event Trigger 7 Register
0x180	MXCCtrl0	UINT32	Multiplexed Counter 0 Control Register
0x184	MXCPresc0	UINT32	Multiplexed Counter 0 Prescaler Register
0x188	MXCCtrl1	UINT32	Multiplexed Counter 1 Control Register
0x18C	MXCPresc1	UINT32	Multiplexed Counter 1 Prescaler Register
0x190	MXCCtrl2	UINT32	Multiplexed Counter 2 Control Register
0x194	MXCPresc2	UINT32	Multiplexed Counter 2 Prescaler Register
0x198	MXCCtrl3	UINT32	Multiplexed Counter 3 Control Register
0x19C	MXCPresc3	UINT32	Multiplexed Counter 3 Prescaler Register

0x1A0	MXCCtrl4	UINT32	Multiplexed Counter 4 Control Register
0x1A4	MXCPresc4	UINT32	Multiplexed Counter 4 Prescaler Register
0x1A8	MXCCtrl5	UINT32	Multiplexed Counter 5 Control Register
0x1AC	MXCPresc5	UINT32	Multiplexed Counter 5 Prescaler Register
0x1B0	MXCCtrl6	UINT32	Multiplexed Counter 6 Control Register
0x1B4	MXCPresc6	UINT32	Multiplexed Counter 6 Prescaler Register
0x1B8	MXCCtrl7	UINT32	Multiplexed Counter 7 Control Register
0x1BC	MXCPresc7	UINT32	Multiplexed Counter 7 Prescaler Register
0x400	FPOutMap0	UINT16	Front Panel Output 0 Mapping Register
0x402	FPOutMap1	UINT16	Front Panel Output 1 Mapping Register
0x404	FPOutMap2	UINT16	Front Panel Output 2 Mapping Register
0x406	FPOutMap3	UINT16	Front Panel Output 3 Mapping Register
0x440	UnivOutMap0	UINT16	Universal Output 0 Mapping Register
0x442	UnivOutMap1	UINT16	Universal Output 1 Mapping Register
0x444	UnivOutMap2	UINT16	Universal Output 2 Mapping Register
0x446	UnivOutMap3	UINT16	Universal Output 3 Mapping Register
0x448	UnivOutMap4	UINT16	Universal Output 4 Mapping Register
0x44A	UnivOutMap5	UINT16	Universal Output 5 Mapping Register
0x44C	UnivOutMap6	UINT16	Universal Output 6 Mapping Register
0x44E	UnivOutMap7	UINT16	Universal Output 7 Mapping Register
0x450	UnivOutMap8	UINT16	Universal Output 8 Mapping Register
0x452	UnivOutMap9	UINT16	Universal Output 9 Mapping Register
0x500	FPIInMap0	UINT32	Front Panel Input 0 Mapping Register
0x504	FPIInMap1	UINT32	Front Panel Input 1 Mapping Register
0x540	UnivInMap0	UINT32	Front Panel Universal Input 0 Map Register
0x544	UnivInMap1	UINT32	Front Panel Universal Input 1 Map Register
0x548	UnivInMap2	UINT32	Front Panel Universal Input 2 Map Register
0x54C	UnivInMap3	UINT32	Front Panel Universal Input 3 Map Register
0x550	UnivInMap4	UINT32	Front Panel Universal Input 4 Map Register
0x554	UnivInMap5	UINT32	Front Panel Universal Input 5 Map Register
0x558	UnivInMap6	UINT32	Front Panel Universal Input 6 Map Register
0x55C	UnivInMap7	UINT32	Front Panel Universal Input 7 Map Register
0x560	UnivInMap8	UINT32	Front Panel Universal Input 8 Map Register
0x564	UnivInMap9	UINT32	Front Panel Universal Input 9 Map Register
0x600	TBInMap0	UINT32	Transition Board Input 0 Mapping Register
0x604	TBInMap1	UINT32	Transition Board Input 1 Mapping Register
0x608	TBInMap2	UINT32	Transition Board Input 2 Mapping Register
0x60C	TBInMap3	UINT32	Transition Board Input 3 Mapping Register
0x610	TBInMap4	UINT32	Transition Board Input 4 Mapping Register
0x614	TBInMap5	UINT32	Transition Board Input 5 Mapping Register
0x618	TBInMap6	UINT32	Transition Board Input 6 Mapping Register
0x61C	TBInMap7	UINT32	Transition Board Input 7 Mapping Register
0x620	TBInMap8	UINT32	Transition Board Input 8 Mapping Register
0x624	TBInMap9	UINT32	Transition Board Input 9 Mapping Register

0x628	TBInMap10	UINT32	Transition Board Input 10 Mapping Register
0x62C	TBInMap11	UINT32	Transition Board Input 11 Mapping Register
0x630	TBInMap12	UINT32	Transition Board Input 12 Mapping Register
0x634	TBInMap13	UINT32	Transition Board Input 13 Mapping Register
0x638	TBInMap14	UINT32	Transition Board Input 14 Mapping Register
0x63C	TBInMap15	UINT32	Transition Board Input 15 Mapping Register
0x800 – 0xFFFF	DataBuf		Data Buffer Transmit Memory
0x1000 – 0x10FF	configROM		
0x1100 – 0x11FF	scratchRAM		
0x1200 – 0x12FF	SFEEPROM		SFP Transceiver EEPROM contents (SFP address 0xA0)
0x1300 – 0x13FF	SFPDIAG		SFP Transceiver diagnostics (SFP address 0xA2)
0x8000 – 0xBFFF	SeqRam0		Sequence RAM 0
0xC000 – 0xFFFF	SeqRam1		Sequence RAM 1

## Status Register

address	bit 31	bit 30	bit 29	Bit 28	bit 27	bit 26	bit 25	bit 24
0x000	RDB7	RDB6	RDB5	RDB4	RDB3	RDB2	RDB1	RDB0

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x001	TDB7	TDB6	TDB5	TDB4	TDB3	TDB2	TDB1	TDB0

Bit	Function
RDB7	Status of received distributed bus bit 7 (from upstream EVG)
RDB6	Status of received distributed bus bit 6 (from upstream EVG)
RDB5	Status of received distributed bus bit 5 (from upstream EVG)
RDB4	Status of received distributed bus bit 4 (from upstream EVG)
RDB3	Status of received distributed bus bit 3 (from upstream EVG)
RDB2	Status of received distributed bus bit 2 (from upstream EVG)
RDB1	Status of received distributed bus bit 1 (from upstream EVG)
RDB0	Status of received distributed bus bit 0 (from upstream EVG)
TDB7	Status of transmitted distributed bus bit 7
TDB6	Status of transmitted distributed bus bit 6
TDB5	Status of transmitted distributed bus bit 5
TDB4	Status of transmitted distributed bus bit 4
TDB3	Status of transmitted distributed bus bit 3
TDB2	Status of transmitted distributed bus bit 2
TDB1	Status of transmitted distributed bus bit 1
TDB0	Status of transmitted distributed bus bit 0

## Control Register

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x004	EVGEN	RXDIS	RXPWD	FIFORS		SRST	LEMDE	MXCRES

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x005								SRALT

Bit	Function
EVGEN	Event Generator Master enable
RXDIS	Disable event reception
RXPWD	Receiver Power down
FIFORS	Reset RX Event Fifo
SRST	Soft reset IP
LEMDE	Little endian mode (cPCI-EVG-300) 0 – PCI core in big endian mode (power up default) 1 – PCI core in little endian mode
MXCRES	Write 1 to reset multiplexed counters
SRALT	(reserved)

## Interrupt Flag Register

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x008								

address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x00a			IFSSTO1	IFSSTO0			IFSSTA1	IFSSTA0

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x00b		IFEXT	IFDBUF				IFFF	IFVIO

Bit	Function
IFSSTO1	Sequence RAM 1 sequence stop interrupt flag
IFSSTO0	Sequence RAM 0 sequence stop interrupt flag
IFSSTA1	Sequence RAM 1 sequence start interrupt flag
IFSSTA0	Sequence RAM 0 sequence start interrupt flag
IFEXT	External Interrupt flag
IFDBUF	Data buffer flag
IFFF	RX Event FIFO full flag
IFVIO	Receiver violation flag

## Interrupt Enable Register

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x00c	IRQEN	PCIIE						

address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x00e			IESSTO1	IESSTO0			IESSTA1	IESSTA0

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x00f		IEEXT	IEDBUF				IEFF	IEVIO

Bit	Function
IRQEN	Master interrupt enable
PCIIE	PCI core interrupt enable (cPCI-EVG-300)
	This bit is used by the low level driver to disable further interrupts before the first interrupt has been handled in user space
IESSTO1	Sequence RAM 1 sequence stop interrupt enable
IESSTO0	Sequence RAM 0 sequence stop interrupt enable
IESSTA1	Sequence RAM 1 sequence start interrupt enable
IESSTA0	Sequence RAM 0 sequence start interrupt enable
IEEXT	External interrupt enable
IEDBUF	Data buffer interrupt enable
IEFF	Event FIFO full interrupt enable
IEVIO	Receiver violation interrupt enable

### AC Trigger Control Register

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x011							ACBYP	ACSYNC

address	bit 15	Bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x012	AC Trigger Divider							

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x013	AC Trigger Phase Shift							

Bit	Function
ACBYP	AC divider and phase shifter bypass (0 = divider/phase shifter enabled, 1 = divider/phase shifter bypassed)
ACSYNC	Synchronization select (0 = event clock, 1 = multiplexed counter 7 output)

### AC Trigger Mapping Register

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x017	ACM7	ACM6	ACM5	ACM4	ACM3	ACM2	ACM1	ACM0

Bit	Function
ACM7	If set AC circuit triggers Event Trigger 7
ACM6	If set AC circuit triggers Event Trigger 6
ACM5	If set AC circuit triggers Event Trigger 5
ACM4	If set AC circuit triggers Event Trigger 4
ACM3	If set AC circuit triggers Event Trigger 3
ACM2	If set AC circuit triggers Event Trigger 2
ACM1	If set AC circuit triggers Event Trigger 1
ACM0	If set AC circuit triggers Event Trigger 0

## Software Event Register

address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x01A							SWPEND	SWENA

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x01B	Event Code to be sent out							

**Bit      Function**

SWPEND Event code waiting to be sent out (read-only). A new event code may be written to the event code register when this bit reads '0'.

SWENA Enable software event

## Data Buffer Control Register

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x021				TXCPT	TXRUN	TRIG	ENA	MODE

address	bit 15	Bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x022							DTSZ(10:8)	

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x023	DTSZ(7:2)							

**Bits      Function**

TXCPT Data Buffer Transmission Complete

TXRUN Data Buffer Transmission Running – set when data transmission has been triggered and has not been completed yet

TRIG Data Buffer Trigger Transmission

Write '1' to start transmission of data in buffer

ENA Data Buffer Transmission enable

'0' – data transmission engine disabled

'1' – data transmission engine enabled

MODE Distributed bus sharing mode

'0' – distributed bus not shared with data transmission

'1' – distributed bus shared with data transmission

DTSZ(10:8) Data Transfer size 4 bytes to 2k in four byte increments

## Distributed Bus Mapping Register

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x024	DBMAP7(3:0)				DBMAP6(3:0)			

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x025							DBMAP4(3:0)	

address	bit 15	Bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x026							DBMAP2(3:0)	

address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x027				DBMAP1(3:0)				DBMAP0(3:0)

Bits	Function
DBMAP7(3:0)	Distributed Bus Bit 7 Mapping: 0 – Off, output logic ‘0’ 1 – take bus bit from external input 2 – Multiplexed counter output mapped to distributed bus bit 3 – Distributed bus bit forwarded from upstream EVG
DBMAP6(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)
DBMAP5(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)
DBMAP4(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)
DBMAP3(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)
DBMAP2(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)
DBMAP1(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)
DBMAP0(3:0)	Distributed Bus Bit 7 Mapping (see above for mappings)

### Distributed Bus Event Enable Register

address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x02B	DBEV7	DBEV6	DBEV5					

Bits	Function
DBEV5	Distributed bus input 5 “Timestamp reset” 0x7D event enable
DBEV6	Distributed bus input 6 “Seconds ‘0’” 0x70 event enable
DBEV7	Distributed bus input 7 “Seconds ‘1’” 0x71 event enable

### FPGA Firmware Version Register

address	bit 31	bit 27	bit 26	bit 24
0x02C		EVG = 0x2		Form Factor
address	bit 23			bit 8
0x02D			Reserved	
address	bit 7			bit 0
0x02F			Version ID	

Bits	Function
Form Factor	0 – CompactPCI 3U 1 – PMC 2 – VME64x 3 – CompactRIO 4 – CompactPCI 6U 6 – PXIE

7 – PCIe

### Timestamp Generator Control Register

address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x037							TSGENA	TSGLOAD

Bits	Function
TSGENA	Timestamp Generator Enable ('0' = disable, '1' = enable)
TSGLOAD	Timestamp Generator Load new value into Timestamp Counter Write '1' to load new value

### Microsecond Divider Register

address	bit 15	bit 0
0x04e		Rounded integer value of 1 $\mu$ s * event clock

For 100 MHz event clock this register should read 100, for 50 MHz event clock this register should read 50. This value is used e.g. for the phase shifter in the AC input logic.

### Clock Control Register

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x050						RFSEL2	RFSEL1	RFSEL0
address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x051			RFDIV5	RFDIV4	RFDIV3	RFDIV2	RFDIV1	RFDIV0
address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x052	RECDCM RUN	RECDCM INITDONE	RECDCM PSDONE	EVDCM STOPPED	EVDCM LOCKED	EVDCM PSDONE	CGLOCK	RECDCM PSDEC
address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x053	RECDCM PSINC	RECDCM RES	EVDCM PSDEC	EVDCM PSINC	EVDCM SRUN	EVDCM SRES	EVDCM RES	RXCLKSEL

Bit	Function
RFDIV5-0	External RF divider select: 000000 – RF/1 000001 – RF/2 000010 – RF/3 000011 – RF/4 000100 – RF/5 000101 – RF/6 000110 – RF/7 000111 – RF/8 001000 – RF/9 001001 – RF/10 001010 – RF/11 001011 – RF/12

	001100 – OFF
	001101 – RF/14
	001110 – RF/15
	001111 – RF/16
	010000 – RF/17
	010001 – RF/18
	010010 – RF/19
	010011 – RF/20
	010100 – RF/21
	010101 – RF/22
	010110 – RF/23
	010111 – RF/24
	011000 – RF/25
	011001 – RF/26
	011010 – RF/27
	011011 – RF/28
	011100 – RF/29
	011101 – RF/30
	011110 – RF/31
	011111 – RF/32
RFSEL2-0	RF reference select: 000 – Use internal reference (fractional synthesizer) 001 – Use external RF reference (front panel input through divider) 010 – PXIe 100 MHz clock 100 – Use recovered RX clock 110 – PXIe 10 MHz clock through clock multiplier
CGLOCK	Micrel SY87739L locked (read-only)

## Event Analyser Control Register

address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x063				EVANE	EVARS	EVAOF	EVAEN	EVACR

Bits	Function
EVANE	Event Analyser FIFO not empty flag: 0 – FIFO empty 1 – FIFO not empty, events in FIFO
EVARS	Event Analyser Reset 0 – not in reset 1 – reset
EVAOF	Event Analyser FIFO overflow flag: 0 – no overflow 1 – FIFO overflow
EVAEN	Event Analyser enable 0 – Event Analyser disabled 1 – Event Analyser enabled

EVACR      Event Analyser 64 bit counter reset  
 0 – Counter running  
 1 – Counter reset to zero.

### Event Analyser Data Register

address	bit 15	bit 8	bit 7	bit 0
0x066	(reserved)			Event Code

### Event Analyser Counter Registers

address	bit 31	bit 0
0x068	Event Analyser Counter Register (bits 63 – 32)	
address	bit 31	bit 0
0x06C	Event Analyser Counter Register (bits 31 – 0)	

### Sequence RAM Control Registers

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x070							SQ0RUN	SQ0ENA
address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x071	SQ0XTR	SQ0XEN	SQ0SWT	SQ0SNG	SQ0REC	SQ0RES	SQ0DIS	SQ0EN
address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x072								
address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x073					SQ0TSEL			
address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x074							SQ1RUN	SQ1ENA
address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x075	SQ1XTR	SQ1XEN	SQ1SWT	SQ1SNG	SQ1REC	SQ1RES	SQ1DIS	SQ1EN
Address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x076								
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x077					SQ1TSEL			

Bit	Function
SQxRUN	Sequence RAM running flag (read-only)
SQxENA	Sequence RAM enabled flag (read_only)
SQxSWT	Sequence RAM software trigger, write '1' to trigger
SQxSNG	Sequence RAM single mode
SQxREC	Sequence RAM recycle mode

SQxRES	Sequence RAM reset, write '1' to reset
SQxDIS	Sequence RAM disable, write '1' to disable
SQxEN	Sequence RAM enable, write '1' to enable/arm
SQxXEN	Sequence RAM allow external enable, '1' - allow
SQxXTR	Sequence RAM allow external trigger enable, '1' - allow
SQxTSEL	Sequence RAM trigger select: 0 – trigger from MXC0 1 – trigger from MXC1 2 – trigger from MXC2 3 – trigger from MXC3 4 – trigger from MXC4 5 – trigger from MXC5 6 – trigger from MXC6 7 – trigger from MXC7 16 – trigger from AC synchronization logic 17 – trigger from sequence RAM 0 software trigger 18 – trigger from sequence RAM 1 software trigger 24 – trigger from sequence RAM 0 external trigger 25 – trigger from sequence RAM 1 external trigger 31 – trigger disabled (default after power up)

## SY87739L Fractional Divider Configuration Word

**address** **bit 31** **bit 0**  
0x080 SY87739L Fractional Divider Configuration Word

Configuration Word	Frequency with 24 MHz reference oscillator
0x0C928166	124.907 MHz
0x0C9282A6	62.454 MHz
0x009743AD	50 MHz
0xC25B43AD	49.978 MHz
0x0176C36D	49.965 MHz

## Event Trigger Registers

Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x103					EVCD0(7:0)			

Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x107					EVCD1(7:0)			

Address bit 15 bit 14 bit 13 bit 12 bit 11 bit 10 bit 9 bit 8

0x10A								EVEN2
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x10B					EVCD2(7:0)			
Address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x10E								EVEN3
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x10F					EVCD3(7:0)			
Address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x102								EVEN4
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x103					EVCD4(7:0)			
Address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x106								EVEN5
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x107					EVCD5(7:0)			
Address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x10A								EVEN6
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x10B					EVCD6(7:0)			
Address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x10E								EVEN7
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x10F					EVCD7(7:0)			

Bit	Function
EVENx	Enable Event Trigger x
EVCDx	Event Trigger Code for Event trigger x

## Multiplexed Counter Registers

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x180	MXC0	MXP0						
address	Bit 7	bit 6	bit 5	Bit 4	Bit 3	bit 2	bit 1	bit 0
0x183	MX0EV7	MX0EV6	MX0EV5	MX0EV4	MX0EV3	MX0EV2	MX0EV1	MX0EV0
address	bit 31							bit 0

0x184	Multiplexed Counter 0 prescaler							
address	<b>bit 31</b>	<b>bit 30</b>	<b>bit 29</b>	<b>bit 28</b>	<b>bit 27</b>	<b>bit 26</b>	<b>bit 25</b>	<b>bit 24</b>
0x188	MXC1	MXP1						
address	<b>Bit 7</b>	<b>bit 6</b>	<b>bit 5</b>	<b>Bit 4</b>	<b>Bit 3</b>	<b>bit 2</b>	<b>bit 1</b>	<b>bit 0</b>
0x18B	MX1EV7	MX1EV6	MX1EV5	MX1EV4	MX1EV3	MX1EV2	MX1EV1	MX1EV0
address	<b>bit 31</b>							
0x18C	Multiplexed Counter 1 prescaler							
Address	<b>bit 31</b>	<b>bit 30</b>	<b>bit 29</b>	<b>bit 28</b>	<b>bit 27</b>	<b>bit 26</b>	<b>bit 25</b>	<b>bit 24</b>
0x190	MXC2	MXP2						
Address	<b>Bit 7</b>	<b>bit 6</b>	<b>bit 5</b>	<b>Bit 4</b>	<b>Bit 3</b>	<b>bit 2</b>	<b>bit 1</b>	<b>bit 0</b>
0x193	MX2EV7	MX2EV6	MX2EV5	MX2EV4	MX2EV3	MX2EV2	MX2EV1	MX2EV0
address	<b>bit 31</b>							
0x194	Multiplexed Counter 2 prescaler							
Address	<b>bit 31</b>	<b>bit 30</b>	<b>bit 29</b>	<b>bit 28</b>	<b>bit 27</b>	<b>bit 26</b>	<b>bit 25</b>	<b>bit 24</b>
0x198	MXC3	MXP3						
Address	<b>Bit 7</b>	<b>bit 6</b>	<b>bit 5</b>	<b>Bit 4</b>	<b>Bit 3</b>	<b>bit 2</b>	<b>bit 1</b>	<b>bit 0</b>
0x19B	MX3EV7	MX3EV6	MX3EV5	MX3EV4	MX3EV3	MX3EV2	MX3EV1	MX3EV0
address	<b>bit 31</b>							
0x19C	Multiplexed Counter 3 prescaler							
Address	<b>bit 31</b>	<b>bit 30</b>	<b>bit 29</b>	<b>bit 28</b>	<b>bit 27</b>	<b>bit 26</b>	<b>bit 25</b>	<b>bit 24</b>
0x1A0	MXC4	MXP4						
Address	<b>Bit 7</b>	<b>bit 6</b>	<b>bit 5</b>	<b>Bit 4</b>	<b>Bit 3</b>	<b>bit 2</b>	<b>bit 1</b>	<b>bit 0</b>
0x1A3	MX4EV7	MX4EV6	MX4EV5	MX4EV4	MX4EV3	MX4EV2	MX4EV1	MX4EV0
address	<b>bit 31</b>							
0x1A4	Multiplexed Counter 4 prescaler							
Address	<b>bit 31</b>	<b>bit 30</b>	<b>bit 29</b>	<b>bit 28</b>	<b>bit 27</b>	<b>bit 26</b>	<b>bit 25</b>	<b>Bit 24</b>
0x1A8	MXC5	MXP5						
Address	<b>Bit 7</b>	<b>bit 6</b>	<b>bit 5</b>	<b>Bit 4</b>	<b>Bit 3</b>	<b>bit 2</b>	<b>bit 1</b>	<b>bit 0</b>
0x1AB	MX5EV7	MX5EV6	MX5EV5	MX5EV4	MX5EV3	MX5EV2	MX5EV1	MX5EV0
address	<b>bit 31</b>							
0x1AC	Multiplexed Counter 5 prescaler							
Address	<b>bit 31</b>	<b>bit 30</b>	<b>bit 29</b>	<b>bit 28</b>	<b>bit 27</b>	<b>bit 26</b>	<b>bit 25</b>	<b>bit 24</b>

0x1B0	MXC6	MXP6						
-------	------	------	--	--	--	--	--	--

Address	Bit 7	bit 6	bit 5	Bit 4	Bit 3	bit 2	bit 1	bit 0
0x1B3	MX6EV7	MX6EV6	MX6EV5	MX6EV4	MX6EV3	MX6EV2	MX6EV1	MX6EV0

address	bit 31	bit 0
0x1B4	Multiplexed Counter 6 prescaler	

Address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x1B8	MXC7	MXP7						

Address	Bit 7	bit 6	bit 5	Bit 4	Bit 3	bit 2	bit 1	bit 0
0x1BB	MX7EV7	MX7EV6	MX7EV5	MX7EV4	MX7EV3	MX7EV2	MX7EV1	MX7EV0

address	bit 31	Bit 0
0x1BC	Multiplexed Counter 7 prescaler	

Bit	Function
MXCx	Multiplexed counter output status (read-only)
MXPx	Multiplexed counter output polarity
MXxEV7	Map rising edge of multiplexed counter x to send out event trigger 7
MXxEV6	Map rising edge of multiplexed counter x to send out event trigger 6
MXxEV5	Map rising edge of multiplexed counter x to send out event trigger 5
MXxEV4	Map rising edge of multiplexed counter x to send out event trigger 4
MXxEV3	Map rising edge of multiplexed counter x to send out event trigger 3
MXxEV2	Map rising edge of multiplexed counter x to send out event trigger 2
MXxEV1	Map rising edge of multiplexed counter x to send out event trigger 1
MXxEV0	Map rising edge of multiplexed counter x to send out event trigger 0

## Front Panel Output Mapping Registers

Address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x401								Front panel OUT0 Mapping ID (see Table 2 for mapping IDs)
0x403								Front panel OUT1 Mapping ID
0x405								Front panel OUT2 Mapping ID
0x407								Front panel OUT3 Mapping ID

Notes:

cPCI-EVG does not have any Front panel outputs.

VME-EVG-230 has four Front panel outputs OUT0 to OUT3.

## Universal Output Mapping Registers

Address	Bit 7	bit 6	bit 5	Bit 4	bit 3	bit 2	bit 1	bit 0
0x441								Universal I/O OUT0 Mapping ID (see Table 2 for mapping IDs)
0x443								Universal I/O OUT1 Mapping ID
0x445								Universal I/O OUT2 Mapping ID
0x447								Universal I/O OUT3 Mapping ID
0x449								Universal I/O OUT4 Mapping ID
0x44B								Universal I/O OUT5 Mapping ID
0x44D								Universal I/O OUT6 Mapping ID
0x44F								Universal I/O OUT7 Mapping ID

0x451	Universal I/O OUT8 Mapping ID
0x453	Universal I/O OUT9 Mapping ID

## Notes:

cPCI-EVG has a maximum of four Universal I/O outputs and six additional outputs are provided by the optional side-by-side module.  
 VME-EVG-230 has a maximum four Universal I/O outputs.

## Front Panel Input Mapping Registers

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x500								FP0IRQ

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x501	FP0DB7	FP0DB6	FP0DB5	FP0DB4	FP0DB3	FP0DB2	FP0DB1	FP0DB0

address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x502			FP0SEN1	FP0SEN0			FP0SEQ1	FP0SEQ0

Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x503	FP0EV7	FP0EV6	FP0EV5	FP0EV4	FP0EV3	FP0EV2	FP0EV1	FP0EV0

address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x505	FP1DB7	FP1DB6	FP1DB5	FP1DB4	FP1DB3	FP1DB2	FP1DB1	FP1DB0

Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x507	FP1EV7	FP1EV6	FP1EV5	FP1EV4	FP1EV3	FP1EV2	FP1EV1	FP1EV0

Bit	Function
FPxIRQ	Map Front panel Input x to External Interrupt
FPxDB7	Map Front panel Input x to Distributed Bus bit 7
FPxDB6	Map Front panel Input x to Distributed Bus bit 6
FPxDB5	Map Front panel Input x to Distributed Bus bit 5
FPxDB4	Map Front panel Input x to Distributed Bus bit 4
FPxDB3	Map Front panel Input x to Distributed Bus bit 3
FPxDB2	Map Front panel Input x to Distributed Bus bit 2
FPxDB1	Map Front panel Input x to Distributed Bus bit 1
FPxDB0	Map Front panel Input x to Distributed Bus bit 0
FPxSEN1	Map Front panel Input x to Sequence External Enable 1
FPxSEN0	Map Front panel Input x to Sequence External Enable 0
FPxSEQ1	Map Front panel Input x to Sequence Trigger 1
FPxSEQ0	Map Front panel Input x to Sequence Trigger 0
FPxEV7	Map Front panel Input x to Event Trigger 7
FPxEV6	Map Front panel Input x to Event Trigger 6
FPxEV5	Map Front panel Input x to Event Trigger 5
FPxEV4	Map Front panel Input x to Event Trigger 4
FPxEV3	Map Front panel Input x to Event Trigger 3
FPxEV2	Map Front panel Input x to Event Trigger 2
FPxEV1	Map Front panel Input x to Event Trigger 1
FPxEV0	Map Front panel Input x to Event Trigger 0

## Universal Input Mapping Registers

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x540								UI0IRQ
address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x541	UI0DB7	UI0DB6	UI0DB5	UI0DB4	UI0DB3	UI0DB2	UI0DB1	UI0DB0
address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8
0x542			UI0SEN1	UI0SEN0			UI0SEQ1	UI0SEQ0
Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x543	UI0EV7	UI0EV6	UI0EV5	UI0EV4	UI0EV3	UI0EV2	UI0EV1	UI0EV0

Bit	Function
UIxIRQ	Map Universal Input x to External Interrupt
UIxDB7	Map Universal Input x to Distributed Bus bit 7
UIxDB6	Map Universal Input x to Distributed Bus bit 6
UIxDB5	Map Universal Input x to Distributed Bus bit 5
UIxDB4	Map Universal Input x to Distributed Bus bit 4
UIxDB3	Map Universal Input x to Distributed Bus bit 3
UIxDB2	Map Universal Input x to Distributed Bus bit 2
UIxDB1	Map Universal Input x to Distributed Bus bit 1
UIxDB0	Map Universal Input x to Distributed Bus bit 0
UIxSEN1	Map Front panel Input x to Sequence External Enable 1
UIxSEN0	Map Front panel Input x to Sequence External Enable 0
UIxSEQ1	Map Front panel Input x to Sequence Trigger 1
UIxSEQ0	Map Front panel Input x to Sequence Trigger 0
UIxEV7	Map Universal Input x to Event Trigger 7
UIxEV6	Map Universal Input x to Event Trigger 6
UIxEV5	Map Universal Input x to Event Trigger 5
UIxEV4	Map Universal Input x to Event Trigger 4
UIxEV3	Map Universal Input x to Event Trigger 3
UIxEV2	Map Universal Input x to Event Trigger 2
UIxEV1	Map Universal Input x to Event Trigger 1
UIxEV0	Map Universal Input x to Event Trigger 0

Note: all enabled input signals are OR'ed together. So if e.g. distributed bus bit 0 has two sources from universal input 0 and 1, if either of the inputs is active high also the distributed bus is active high.

## Transition Board Input Mapping Registers

address	bit 31	bit 30	bit 29	bit 28	bit 27	bit 26	bit 25	bit 24
0x540								TI0IRQ
address	bit 23	bit 22	bit 21	bit 20	bit 19	bit 18	bit 17	bit 16
0x541	TI0DB7	TI0DB6	TI0DB5	TI0DB4	TI0DB3	TI0DB2	TI0DB1	TI0DB0
address	bit 15	bit 14	bit 13	bit 12	bit 11	bit 10	bit 9	bit 8

0x542			TI0SEN1	TI0SEN0			TI0SEQ1	TI0SEQ0
-------	--	--	---------	---------	--	--	---------	---------

Address	bit 7	bit 6	bit 5	bit 4	bit 3	bit 2	bit 1	bit 0
0x543	TI0EV7	TI0EV6	TI0EV5	TI0EV4	TI0EV3	TI0EV2	TI0EV1	TI0EV0

Bit	Function
TIxIRQ	Map Universal Input x to External Interrupt
TIxDB7	Map Universal Input x to Distributed Bus bit 7
TIxDB6	Map Universal Input x to Distributed Bus bit 6
TIxDB5	Map Universal Input x to Distributed Bus bit 5
TIxDB4	Map Universal Input x to Distributed Bus bit 4
TIxDB3	Map Universal Input x to Distributed Bus bit 3
TIxDB2	Map Universal Input x to Distributed Bus bit 2
TIxDB1	Map Universal Input x to Distributed Bus bit 1
TIxDB0	Map Universal Input x to Distributed Bus bit 0
TIxSEN1	Map Front panel Input x to Sequence External Enable 1
TIxSEN0	Map Front panel Input x to Sequence External Enable 0
TIxSEQ1	Map Front panel Input x to Sequence Trigger 1
TIxSEQ0	Map Front panel Input x to Sequence Trigger 0
TIxEV7	Map Universal Input x to Event Trigger 7
TIxEV6	Map Universal Input x to Event Trigger 6
TIxEV5	Map Universal Input x to Event Trigger 5
TIxEV4	Map Universal Input x to Event Trigger 4
TIxEV3	Map Universal Input x to Event Trigger 3
TIxEV2	Map Universal Input x to Event Trigger 2
TIxEV1	Map Universal Input x to Event Trigger 1
TIxEV0	Map Universal Input x to Event Trigger 0

Note: all enabled input signals are OR'ed together. So if e.g. distributed bus bit 0 has two sources from universal input 0 and 1, if either of the inputs is active high also the distributed bus is active high.

## Application Programming Interface (API)

A Linux device driver and application interface is provided to setup up the Event Generator.

### Function Reference

**int EvgOpen(struct MrfEgRegs \*\*pEg, char \*device\_name);**

**Description**

Opens the EVG device for access. Simultaneous accesses are allowed.

**Parameters**      struct MrfEgRegs \*\*pEg

EvgOpen returns pointer to EVG registers by memory mapping the I/O registers into user space.

char \*device\_name

Holds the device name of the EVG, e.g. /dev/ega3. The device names are set up by the module\_load script of the device driver.



**int EvgGetViolation(volatile struct MrfEgRegs \*pEg, int clear);****Description**

Parameters      volatile struct MrfEgRegs \*pEg  
                    int clear

Get/clear EVG RX link violation status.

Pointer to memory mapped EVG register base.

0: don't clear

1: clear status

Returns 0 when no violation detected.

Return value      Return non-zero when violation detected.

**int EvgSWEEventEnable(volatile struct MrfEgRegs \*pEg, int state);****Description**

Parameters      volatile struct MrfEgRegs \*pEg  
                    int state

Enable sending of software event codes.

Pointer to memory mapped EVG register base.

0: disable

1: enable

Returns zero when EVG SW events disabled

Return value      Returns non-zero when EVG SW events enabled

**int EvgGetSWEEventEnable(volatile struct MrfEgRegs \*pEg);****Description**

Parameters      volatile struct MrfEgRegs \*pEg

Retrieve state of software event codes.

Pointer to memory mapped EVG register base.

**Return value**

Returns zero when EVG SW events disabled

Return value      Returns non-zero when EVG SW events enabled

**int EvgSendSWEEvent(volatile struct MrfEgRegs \*pEg, int code);****Description**

Parameters      volatile struct MrfEgRegs \*pEg  
                    int code

Send software event code.

Pointer to memory mapped EVG register base.

Event code to be sent out

Return value      Returns code sent out.

**int EvgEvanEnable(volatile struct MrfEgRegs \*pEg, int state);****Description**

Parameters      volatile struct MrfEgRegs \*pEg  
                    int state

Enable/disable EVG event analyzer.

Pointer to memory mapped EVG register base.

0: disable

1: enable

Returns zero when EVG event analyzer disabled

Return value      Returns non-zero when EVG SW event analyzer enabled

**int EvgEvanGetEnable(volatile struct MrfEgRegs \*pEg);****Description**

Get EVG event analyzer state.

**Parameters**

volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

**Return value**

Returns zero when EVG event analyzer disabled

Returns non-zero when EVG SW event analyzer enabled

**void EvgEvanReset(volatile struct MrfEgRegs \*pEg);****Description**

Reset EVG event analyzer state.

**Parameters**

volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

**Return value**

none

**void EvgEvanResetCount(volatile struct MrfEgRegs \*pEg);****Description**

Reset EVG event analyzer time counter value.

**Parameters**

volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

**Return value**

None

**int EvgEvanGetEvent(volatile struct MrfEgRegs \*pEg, struct EvanStruct \*evan);****Description**

Retrieve one event from event analyzer.

**Parameters**

volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

struct EvanStruct \*evan

Pointer to event analyzer structure to store one event. (see egapi.h for structure details).

**Return value**

Returns zero on success.

Returns -1 if no events available in event analyzer.

**int EvgSetMXCPrescaler(volatile struct MrfEgRegs \*pEg, int mxc, unsigned int presc);****Description**

Set multiplexed counter prescaler.

**Parameters**

volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

int mxc

Multiplexed counter number 0-7.

unsigned int presc

32-bit prescaler value.

**Return value**

Returns zero on success.

Returns -1 on error.

**int EvgSetMxcTrigMap(volatile struct MrfEgRegs \*pEg, int mxc, int map);****Description**

Set multiplexed counter to event trigger mapping.

**Parameters**

Pointer to memory mapped EVG register base.

int mxc

Multiplexed counter number 0-7.

int map

Number of event trigger to map to.

**Return value**

Returns zero on success.

Returns -1 on error.

**void EvgSyncMxc(volatile struct MrfEgRegs \*pEg);****Description**

Synchronize multiplexed counters.

**Parameters**

Pointer to memory mapped EVG register base.

**Return value**

None

**void EvgMXCDump(volatile struct MrfEgRegs \*pEg);****Description**

Dump multiplexed counter registers.

**Parameters**

Pointer to memory mapped EVG register base.

**Return value**

None

**int EvgSetDBusMap(volatile struct MrfEgRegs \*pEg, int dbus, int map);****Description**

Set distributed bus bit mappings.

**Parameters**

Pointer to memory mapped EVG register base.

int dbus

Distributed bus bit number 0-7.

int map

Distributed bus bit source:

C\_EVG\_DBUS\_SEL\_OFF: bit tied to zero

C\_EVG\_DBUS\_SEL\_EXT: external input

C\_EVG\_DBUS\_SEL\_MXC: multiplexed counter

C\_EVG\_DBUS\_SEL\_FORWARD: from upstream EVG

Returns zero on success.

Returns -1 on error.

**Return value****void EvgDBusDump(volatile struct MrfEgRegs \*pEg);****Description**

Dump distributed bus registers.

**Parameters**

Pointer to memory mapped EVG register base.

**Return value** None**int EvgSetACInput(volatile struct MrfEgRegs \*pEg, int bypass, int sync, int div, int delay);****Description** Set AC input parameters.**Parameters** volatile struct MrfEgRegs \*pEg Pointer to memory mapped EVG register base.  
int bypass 0: use AC sync logic  
1: bypass phase shifter and divider  
int sync 0: don't synchronize to MXC7  
1: synchronize to MXC7  
int div Divider 1 – 255  
int delay Phase shift in approx. 0.1 ms steps  
**Return value** Returns zero on success.  
Returns -1 on error.**int EvgSetACMap(volatile struct MrfEgRegs \*pEg, int map);****Description** Set AC input event trigger mapping.**Parameters** volatile struct MrfEgRegs \*pEg Pointer to memory mapped EVG register base.  
int map Number of event trigger to map to.  
**Return value** Returns zero on success.  
Returns -1 on error.**void EvgACDump(volatile struct MrfEgRegs \*pEg);****Description** Dump AC input registers.**Parameters** volatile struct MrfEgRegs \*pEg Pointer to memory mapped EVG register base.  
**Return value** None**int EvgSetRFInput(volatile struct MrfEgRegs \*pEg, int useRF, int div);****Description** Set up event clock RF input.**Parameters** volatile struct MrfEgRegs \*pEg Pointer to memory mapped EVG register base.  
int useRF 0: use internal reference (fractional synthesizer)  
1: use external RF input  
int div C\_EVG\_RFDIV\_1,  
C\_EVG\_RFDIV\_2, etc. see egapi.h for details.  
**Return value** Returns zero on success.  
Returns -1 on error.

**int EvgSetFracDiv(volatile struct MrfEgRegs \*pEg, int fracdiv);****Description**

Set fractional divider control word which provides reference frequency for receiver.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

int fracdiv

Fractional divider control word

**Return value**

Returns control word written

**int EvgSetSeqRamEvent(volatile struct MrfEgRegs \*pEg, int ram, int pos, unsigned int timestamp, int code);****Description**

Write one event into Sequence RAM.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

int ram

Number of Sequence RAM

0: RAM0

1: RAM1

int pos

Event position in memory: 0 – 2047

unsigned int timestamp

Timestamp of event (32-bit)

int code

Event code (8-bit)

**Return value**

Returns zero on success.

Returns -1 on error.

**void EvgSeqRamDump(volatile struct MrfEgRegs \*pEg, int ram);****Description**

Dump Sequence RAM registers.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

**Return value**

None

**int EvgSeqRamControl(volatile struct MrfEgRegs \*pEg, int ram, int enable, int single, int recycle, int reset, int trigsel);****Description**

Setup Sequence RAM

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

int ram

Number of Sequence RAM

0: RAM0

1: RAM1

int enable

0: disable RAM

1: enable RAM

int single

0: multi-sequence

1: single sequence

int recycle

0: trigger mode

1: recycle mode (loop)

int reset

1: reset RAM

int trigsel

See egapi.h

**Return value**

Returns zero on success.

Returns -1 on error.

**int EvgSeqRamSWTrig(volatile struct MrfEgRegs \*pEg, int trig);****Description**

Software trigger Sequence RAM.

**Parameters**Pointer to memory mapped EVG register base.  
volatile struct MrfEgRegs \*pEg  
int trig

0: software trigger 0

1: software trigger 1

Returns 0 on success.

Returns -1 on error.

**Return value****void EvgSeqRamStatus(volatile struct MrfEgRegs \*pEg, int ram);****Description**

Dump Sequence RAM status.

**Parameters**Pointer to memory mapped EVG register base.  
volatile struct MrfEgRegs \*pEg

None

**Return value****int EvgSetUnivinMap(volatile struct MrfEgRegs \*pEg, int univ, int trig, int dbus);****Description**

Set up universal input mappings.

**Parameters**Pointer to memory mapped EVG register base.  
volatile struct MrfEgRegs \*pEg  
int univ  
Number of universal input (0-3 for EVG, 4-9 for side-by-side module)  
int trig  
Number of event trigger to map to.  
int dbus  
Number of external distributed bus input to map to.

Returns 0 on success.

Returns -1 on error.

**Return value****void EvgUnivinDump(volatile struct MrfEgRegs \*pEg);****Description**

Dump Universal input mappings.

**Parameters**Pointer to memory mapped EVG register base.  
volatile struct MrfEgRegs \*pEg

None

**Return value****int EvgSetTriggerEvent(volatile struct MrfEgRegs \*pEg, int trigger, int code, int enable);****Description**

Set up trigger events.

**Parameters**Pointer to memory mapped EVG register base.  
volatile struct MrfEgRegs \*pEg  
int trigger  
Number of trigger event  
int code  
Event code

int enable

0: disable

1: enable

**Return value**

Returns 0 on success.

Returns -1 on error.

**void EvgTriggerEventDump(volatile struct MrfEgRegs \*pEg);****Description**

Dump Event trigger settings.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

**Return value**

None

**int EvgSetUnivOutMap(volatile struct MrfEgRegs \*pEg, int output, int map);****Description**

Set up universal output mappings.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

int output

Universal Output number

int map

Signal mapping (see egapi.h for details)

**Return value**

Returns 0 on success, -1 on error

**int EvgSetDBufMode(volatile struct MrfEgRegs \*pEg, int enable);****Description**

Enable/disable transmitter data buffer mode. When data buffer mode is enabled every other distributed bus byte is reserved for data transmission thus the distributed bus bandwidth is halved.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

int enable

0 – disable transmitter data buffer mode

1 – enable transmitter data buffer mode

Transmit data buffer status (see **Error!****Reference source not found.** on page**Error! Bookmark not defined.** for bit definitions).**int EvgGetDBufStatus(volatile struct MrfEgRegs \*pEg);****Description**

Get transmit data buffer status. When data buffer mode is enabled every other distributed bus byte is reserved for data transmission thus the distributed bus bandwidth is halved.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

**Return value**Transmit data buffer status (see **Error!****Reference source not found.** on page

**Error! Bookmark not defined.** for bit definitions).

**int EvgSendDBuf(volatile struct MrfEgRegs \*pEg, char \*dbuf, int size);****Description**

Get transmit data buffer status. When data buffer mode is enabled every other distributed bus byte is reserved for data transmission thus the distributed bus bandwidth is halved.

**Parameters** volatile struct MrfEgRegs \*pEg

Pointer to memory mapped EVG register base.

char \*dbuf

Pointer to local data buffer

int size

Size of data in bytes to be transmitted:  
4, 8, 12, ..., 2048.

**Return value**

Size of buffer being sent.

-1 on error.